

APPENDIX A

Summary of Results

A1.1

Item 1



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
1	1710.2	512	0	30	Left Head	Cheek

Lab Code	Sample A Result	Sample B Result	Between Laboratories	Within Laboratories	Expanded uncertainty	
	SAR(mW/g)	SAR(mW/g)	Z-Score	Z-Score	Sample A	Sample B
1	0.513	0.437	2.363	0.58	±0.84%	±0.92%
2	0.48	0.432	1.487	-0.298	±23.83%	±23.83%
3	0.465	0.328	-1.256	2.494	±40.6%	±40.6%
4	0.447	0.399	-3.458	-0.298	±20.6%	±20.6%
5	0.398	0.45	1.152	-3.435※	±29.1%	±29.1%
6	0.564	0.445	3.724※	1.929	N/A	N/A
7	0.455	0.375	-0.403	0.705	N/A	N/A
8	0.353	0.331	-3.770※	-1.113	±22.63%	±22.63%
9	0.465	0.424	0.956	-0.517	±20.6%	±20.6%
10	0.43	0.41	-0.172	-1.176	N/A	N/A
11	0.481	0.407	0.933	0.517	±27%	±27%
12	0.401	0.37	-1.764	-0.831	±22%	±22%
13	0.477	0.384	0.311	1.113	±12.61%	±12.61%
14	0.441	0.406	-1.152	-0.705	N/A	N/A
15	0.473	0.405	0.703	0.329	N/A	N/A
16	0.448	0.381	-0.426	0.298	±20.6%	±20.6%


No. of	16	16
Median	0.46	0.405
Normalized IQR	0.029	0.034
Robust CV(%)	6.365	8.5
Maximum	0.564	0.45
Minimum	0.353	0.328
Range	0.211	0.122

NOTE : ※ denotes an outlier (i.e. |z-score| ≥ 3)

A1.2
Item 1 – APLAC Sample A & Sample B

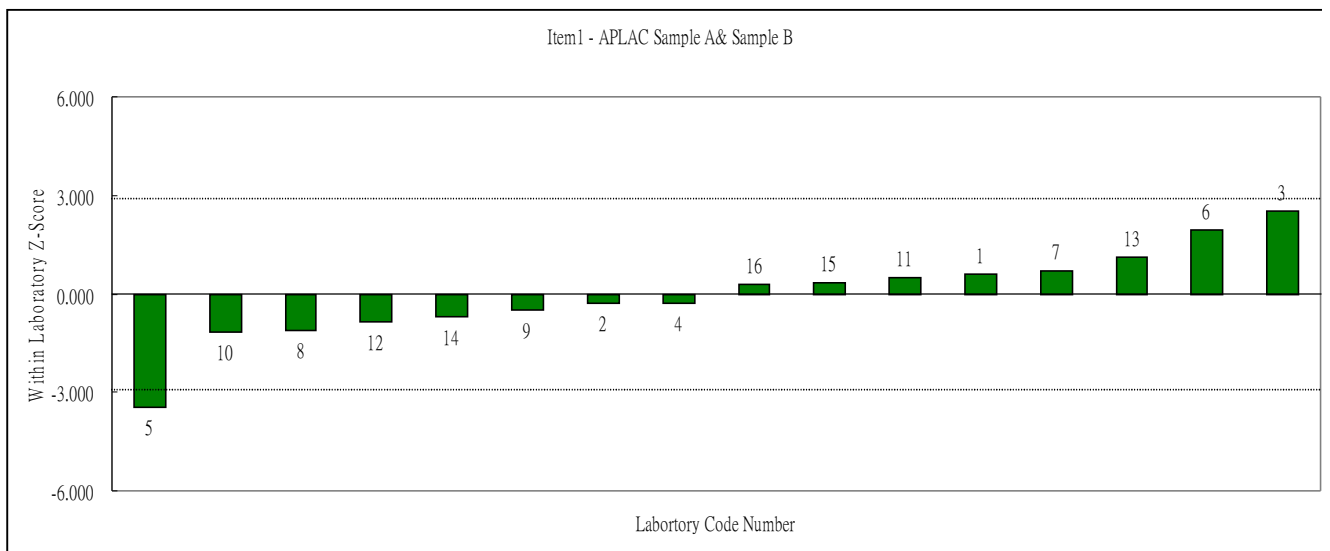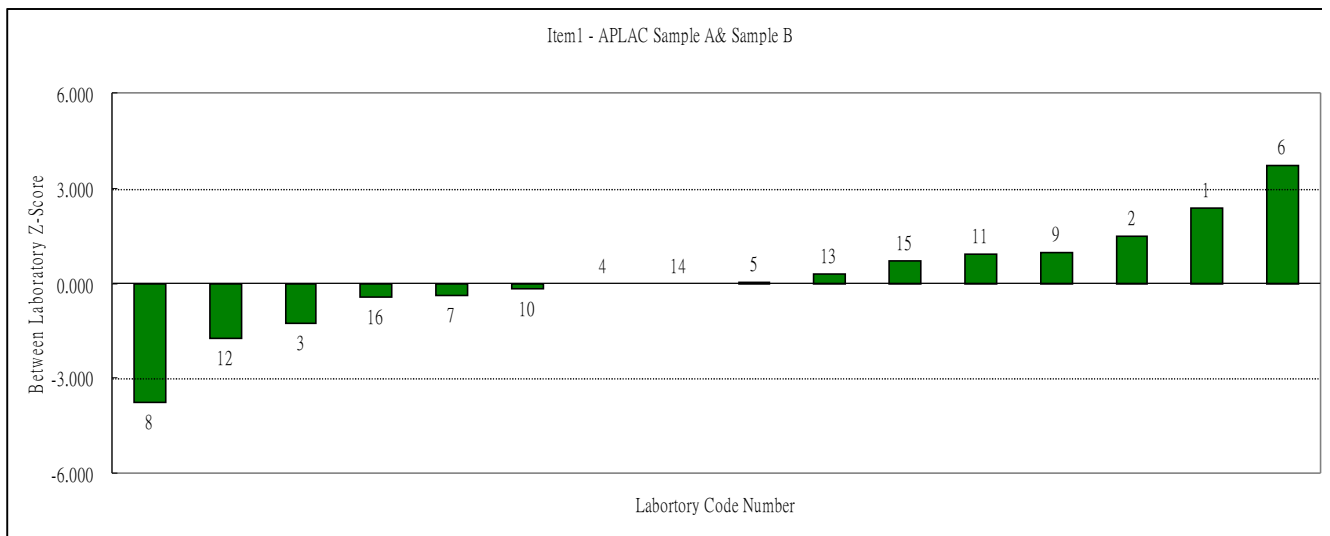

A1.3

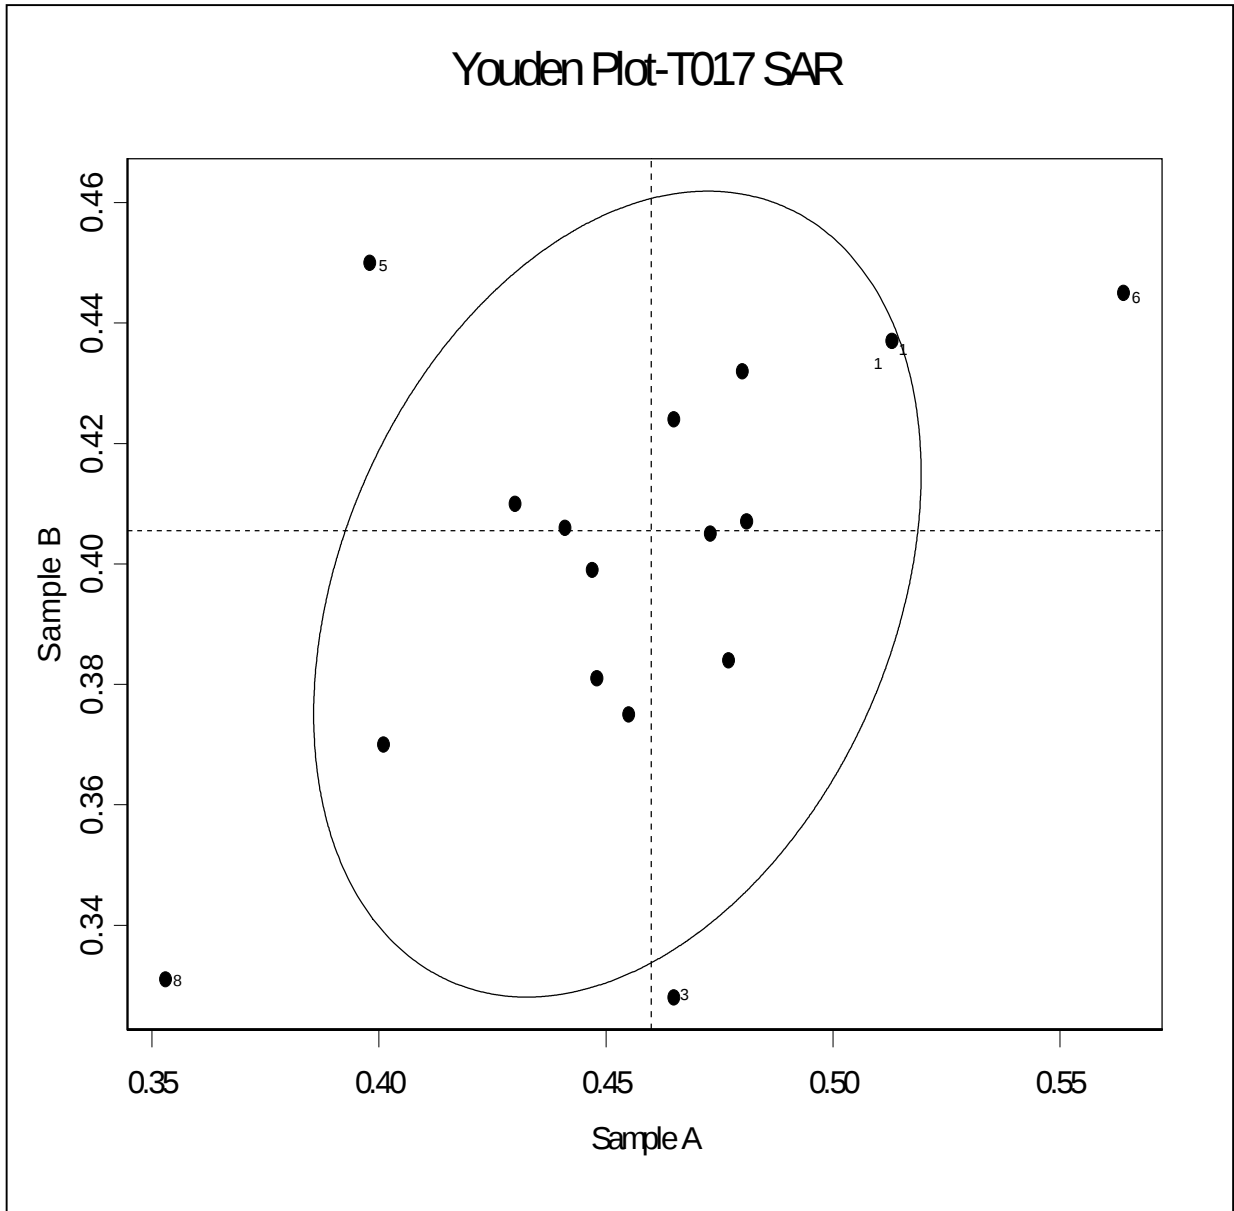

A2.1
Item 2



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
2	1747.8	700	0	30	Left Head	Cheek

Lab Code	Sample A Result	Sample B Result	Between Laboratories	Within Laboratories	Expanded uncertainty	
	SAR(mW/g)	SAR(mW/g)	Z-Score	Z-Score	Sample A	Sample B
1	0.418	0.435	0.62	-0.101	±0.84%	±0.92%
2	0.432	0.445	0.955	-0.37	±23.83%	±23.83%
3	0.415	0.351	-0.592	-5.564※	±40.6%	±40.6%
4	0.388	0.408	-0.174	0.101	±20.6%	±20.6%
5	0.42	0.57	2.53	8.869※	±29.1%	±29.1%
6	0.441	0.455	1.22	-0.303	N/A	N/A
7	0.375	0.387	-0.648	-0.438	N/A	N/A
8	0.261	0.321	-3.158※	2.799	±22.63%	±22.63%
9	0.375	0.383	-0.704	-0.708	±20.6%	±20.6%
10	0.39	0.4	-0.257	-0.573	N/A	N/A
11	0.44	0.478	1.526	1.315	±27%	±27%
12	0.381	0.411	-0.23	0.775	±22%	±22%
13	0.414	0.428	0.467	-0.303	±12.61%	±12.61%
14	0.372	0.403	-0.467	0.843	N/A	N/A
15	0.414	0.453	0.815	1.382	N/A	N/A
16	0.396	0.425	0.174	0.708	±20.6%	±20.6%


No. of	16	16
Median	0.405	0.418
Normalized IQR	0.028	0.037
Robust CV(%)	7.138	8.911
Maximum	0.441	0.57
Minimum	0.261	0.321
Range	0.18	0.249

NOTE : ※ denotes an outlier (i.e. |z-score| ≥ 3)

A2.2
Item 2 – APLAC Sample A & Sample B

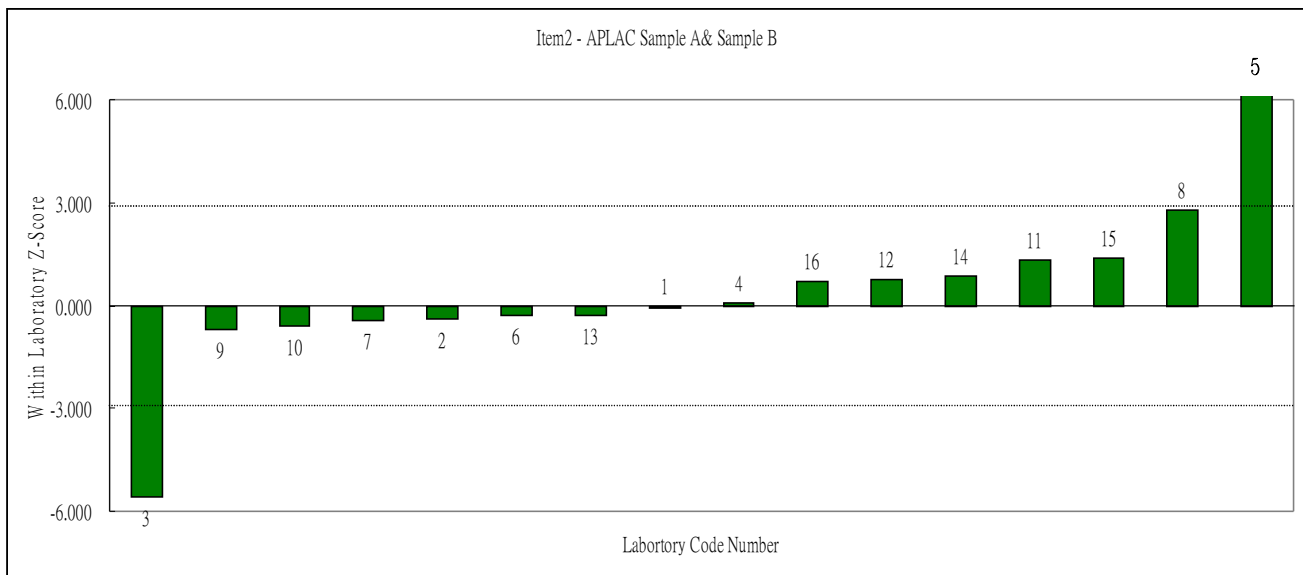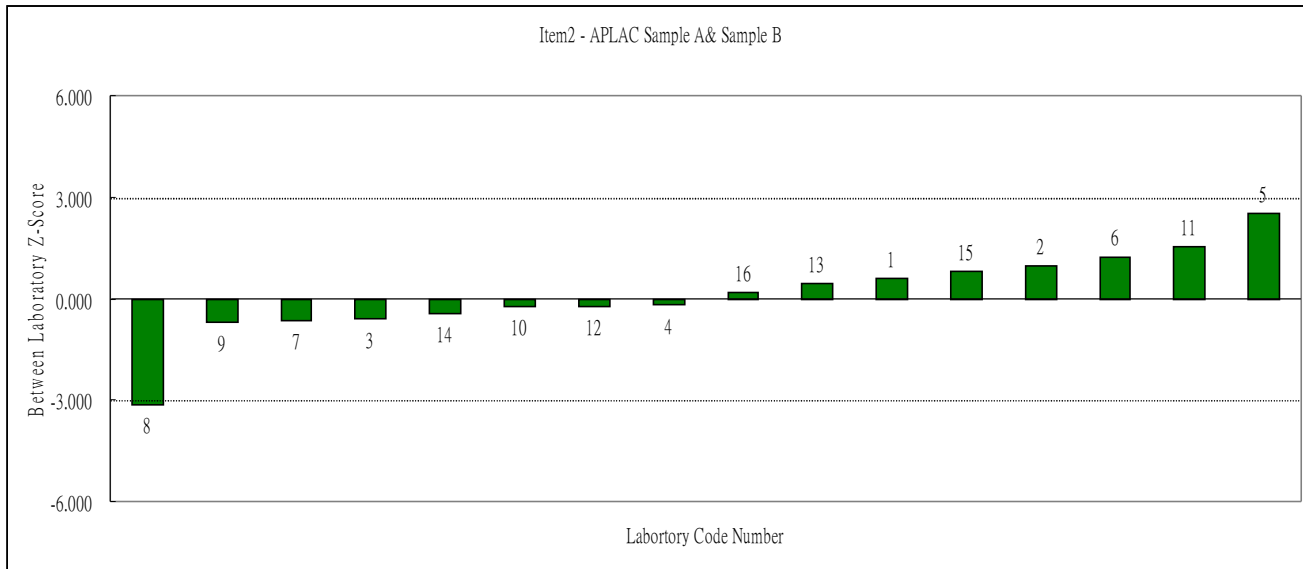

Youden Plot-Concrete

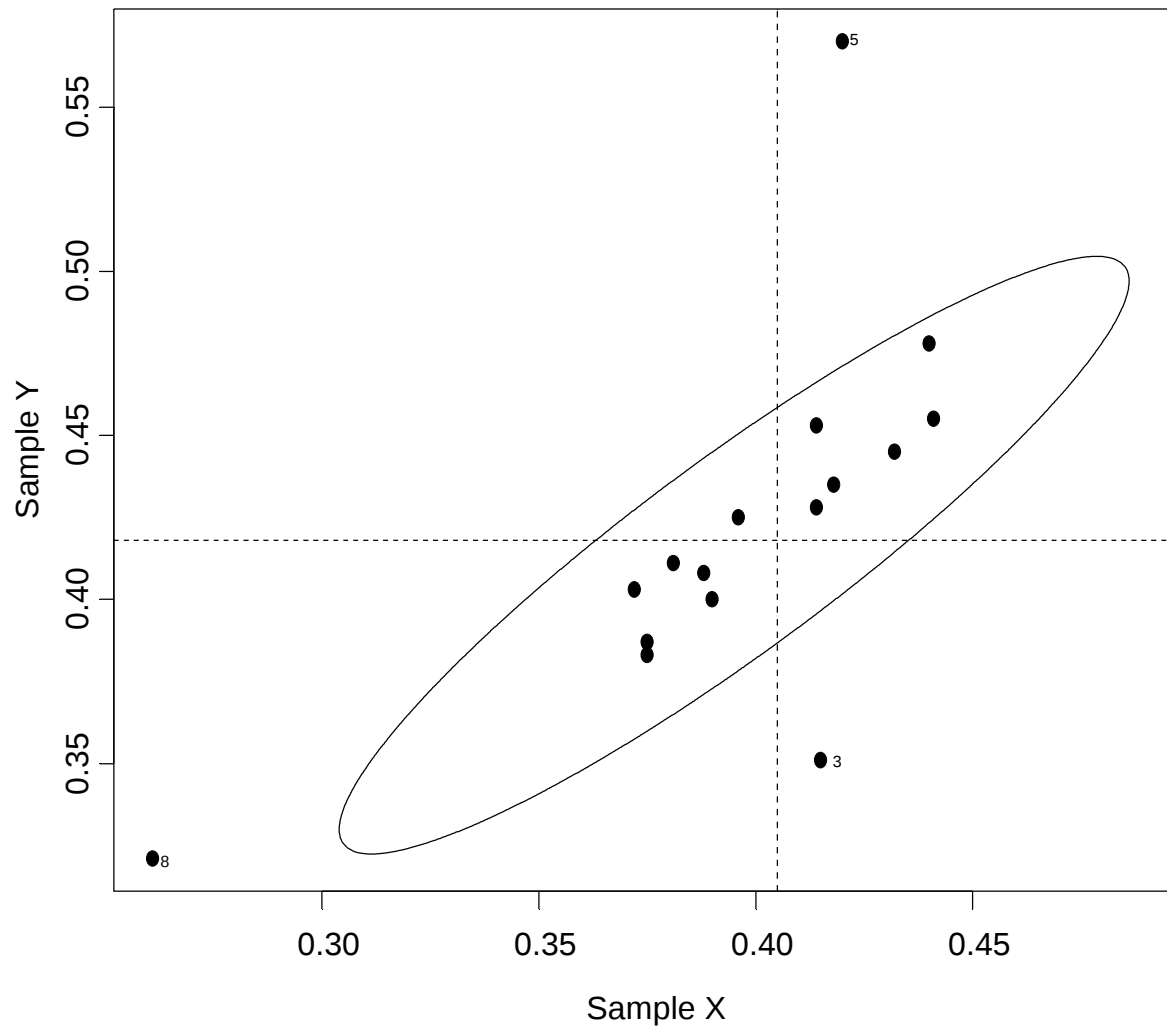

A3.1

Item 3



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
3	1784.8	885	0	30	Left Head	Cheek

Lab Code	Sample A	Sample B	Between Laboratories Z-Score	Within Laboratories Z-Score	Expanded uncertainty	
	Result SAR(mW/g)	Result SAR(mW/g)			Sample A	Sample B
1	0.322	0.342	0.256	0.101	±0.84%	±0.92%
2	0.34	0.366	1.024	0.407	±23.83%	±23.83%
3	0.335	0.268	-0.859	-4.326※	±40.6%	±40.6%
4	0.318	0.327	-9.145	-0.458	±20.6%	±20.6%
5	0.31	0.435	1.737	5.446※	±29.1%	±29.1%
6	0.305	0.351	0.109	1.425	N/A	N/A
7	0.313	0.322	-0.274	-0.458	N/A	N/A
8	0.278	0.291	-1.481	-0.254	±22.63%	±22.63%
9	0.309	0.324	-0.31	-0.152	±20.6%	±20.6%
10	0.37	0.36	1.463	-1.425	N/A	N/A
11	0.327	0.387	1.17	2.138	±27%	±27%
12	0.311	0.329	-0.182	0	±22%	±22%
13	0.299	0.335	-0.292	0.916	±12.61%	±12.61%
14	0.282	0.322	-0.841	1.119	N/A	N/A
15	0.347	0.365	1.134	0	N/A	N/A
16	0.322	0.333	9.145	-0.356	±20.6%	±20.6%


No. of	16	16
Median	0.315	0.334
Normalized IQR	0.015	0.027
Robust CV(%)	4.934	8.378
Maximum	0.37	0.435
Minimum	0.278	0.268
Range	0.092	0.167

NOTE : ※ denotes an outlier (i.e. |z-score| ≥ 3)

A3.2
Item 3 – APLAC Sample A & Sample B

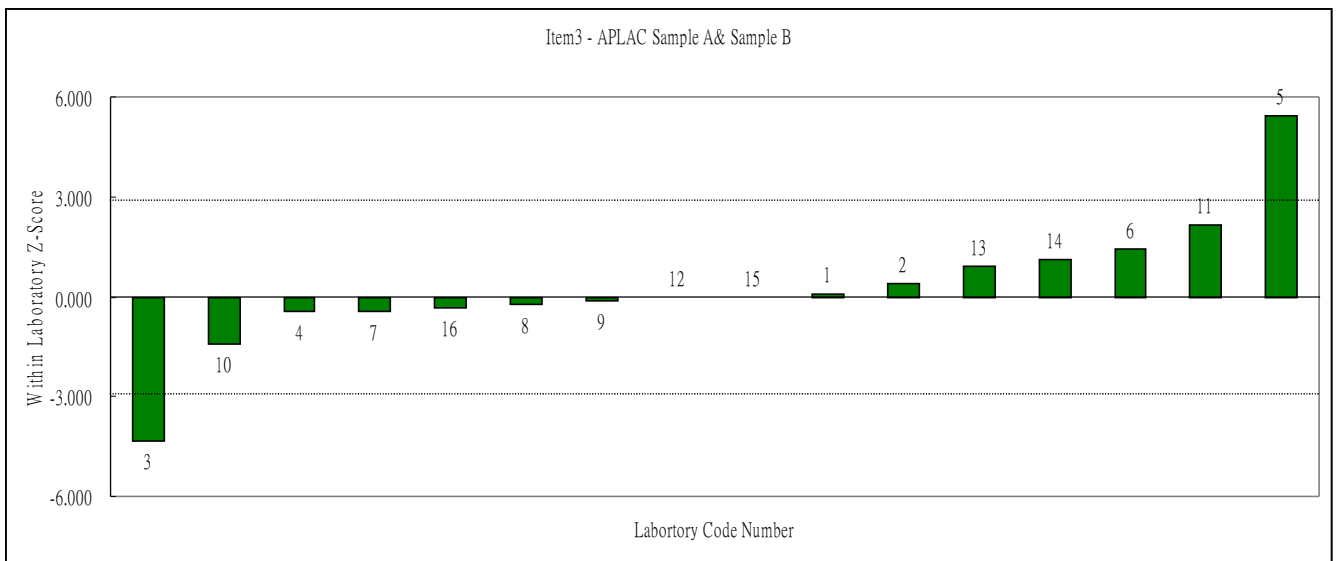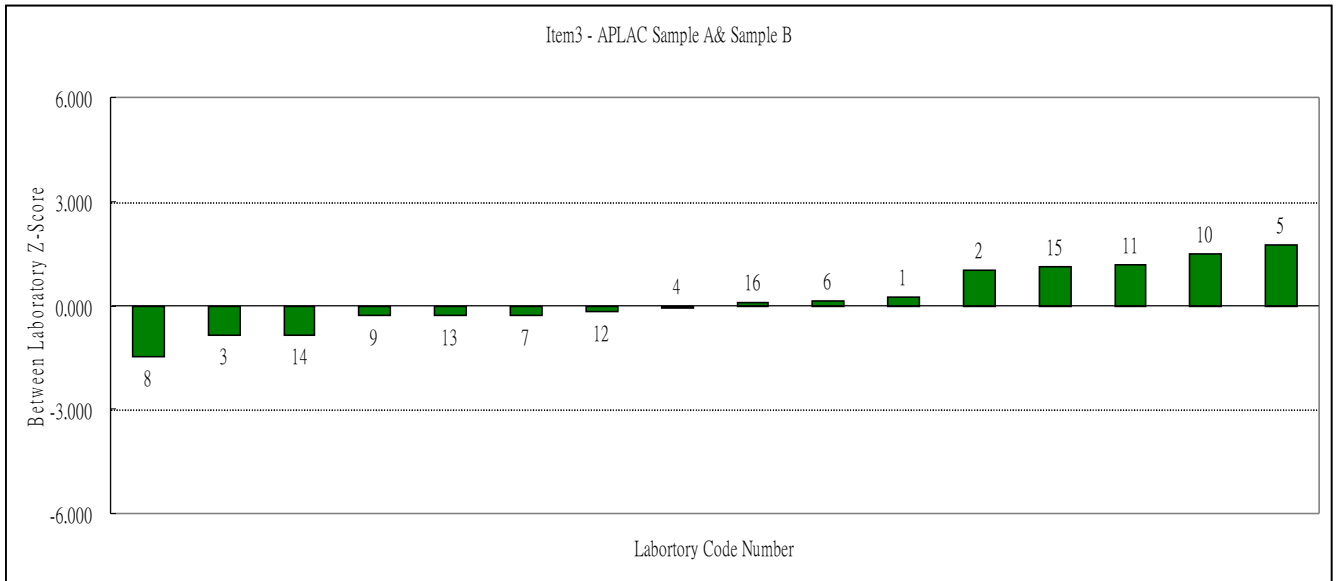

Youden Plot-T017 SAR

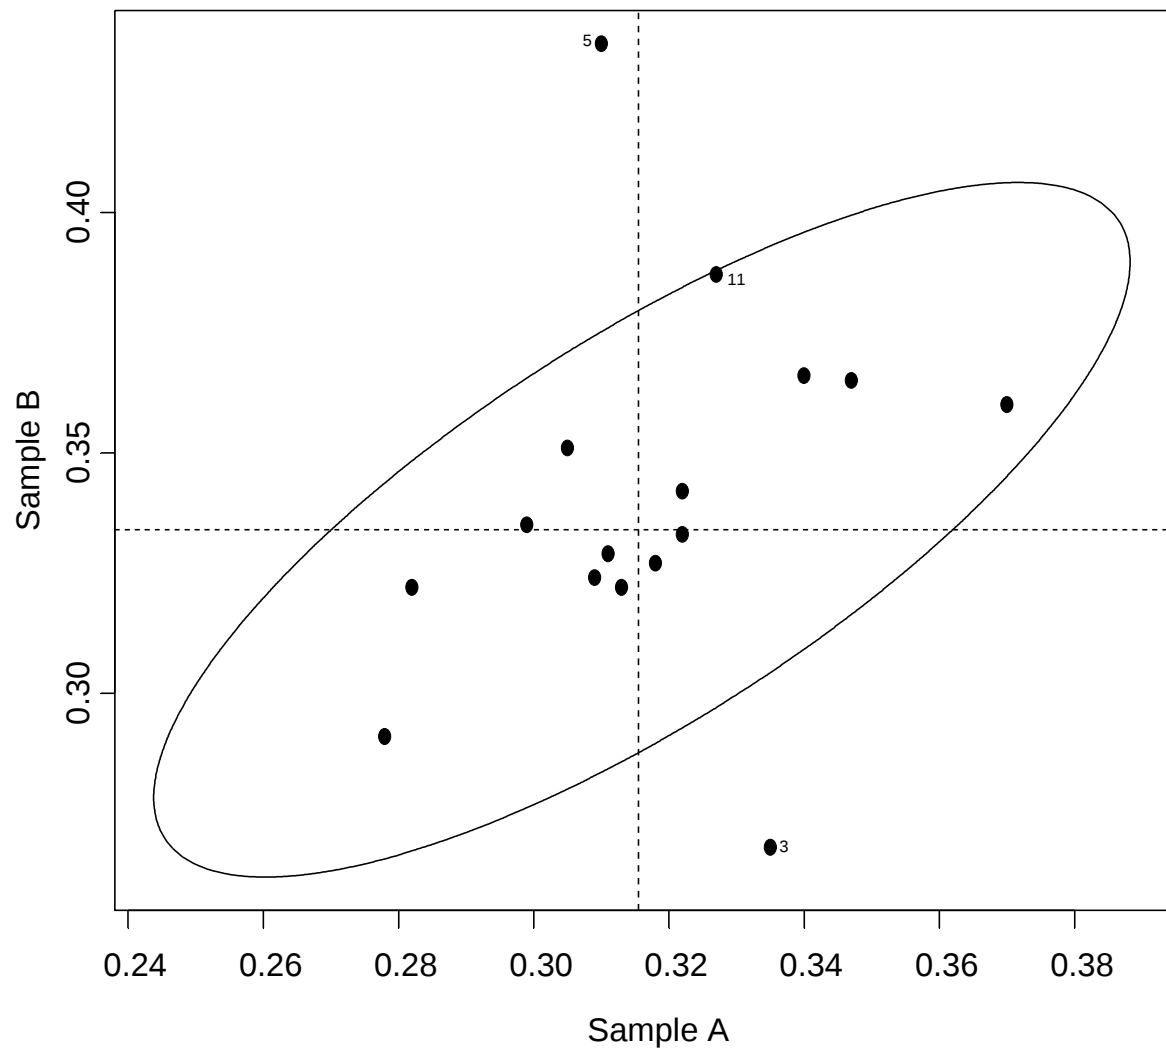

Item 4



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
4	1710.2	512	0	30	Left Head	Tilted 15


Lab Code	Sample A Result	Sample B Result	Between Laboratories	Within Laboratories	Expanded uncertainty	
	SAR(mW/g)	SAR(mW/g)	Z-Score	Z-Score	Sample A	Sample B
1	0.498	0.461	0.789	-0.263	±0.84%	±0.92%
2	0.528	0.46	1.097	0.756	±23.83%	±23.83%
3	0.304	0.273	-3.259※	-0.46	±40.6%	±40.6%
4	0.453	0.412	-0.206	-0.131	±20.6%	±20.6%
5	0.423	0.501	0.418	-4.046※	±29.1%	±29.1%
6	0.412	0.459	-0.143	-3.026※	N/A	N/A
7	0.449	0.379	-0.598	0.822	N/A	N/A
8	0.267	0.303	-3.334※	-2.665	±22.63%	±22.63%
9	0.407	0.407	-0.747	-1.48	±20.6%	±20.6%
10	0.39	0.35	-1.531	-0.164	N/A	N/A
11	0.504	0.446	0.694	0.427	±27%	±27%
12	0.467	0.404	-0.143	0.592	±22%	±22%
13	0.508	0.412	0.376	1.678	±12.61%	±12.61%
14	0.709	0.646	4.987※	0.592	N/A	N/A
15	0.503	0.454	0.768	0.131	N/A	N/A
16	0.483	0.415	0.143	0.756	±20.6%	±20.6%

No. of	16	16
Median	0.46	0.413
Normalized IQR	0.068	0.045
Robust CV(%)	14.906	11.025
Maximum	0.709	0.646
Minimum	0.267	0.273
Range	0.442	0.373

NOTE : ※ denotes an outlier (i.e. |z-score| ≥ 3)

A4.2
Item 4 – APLAC Sample A & Sample B

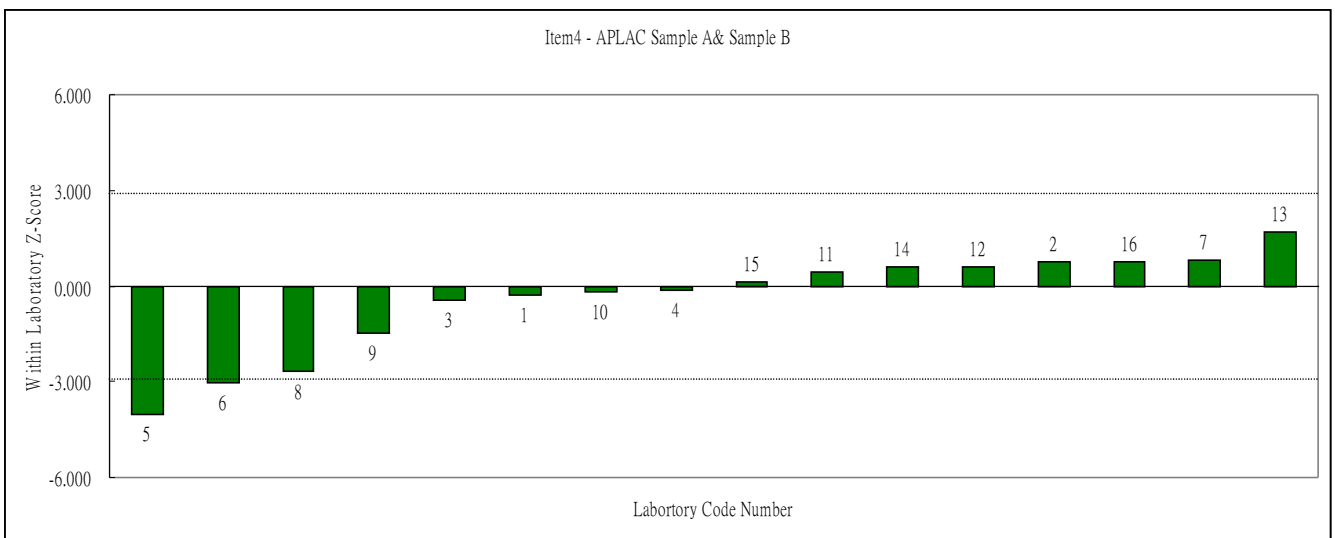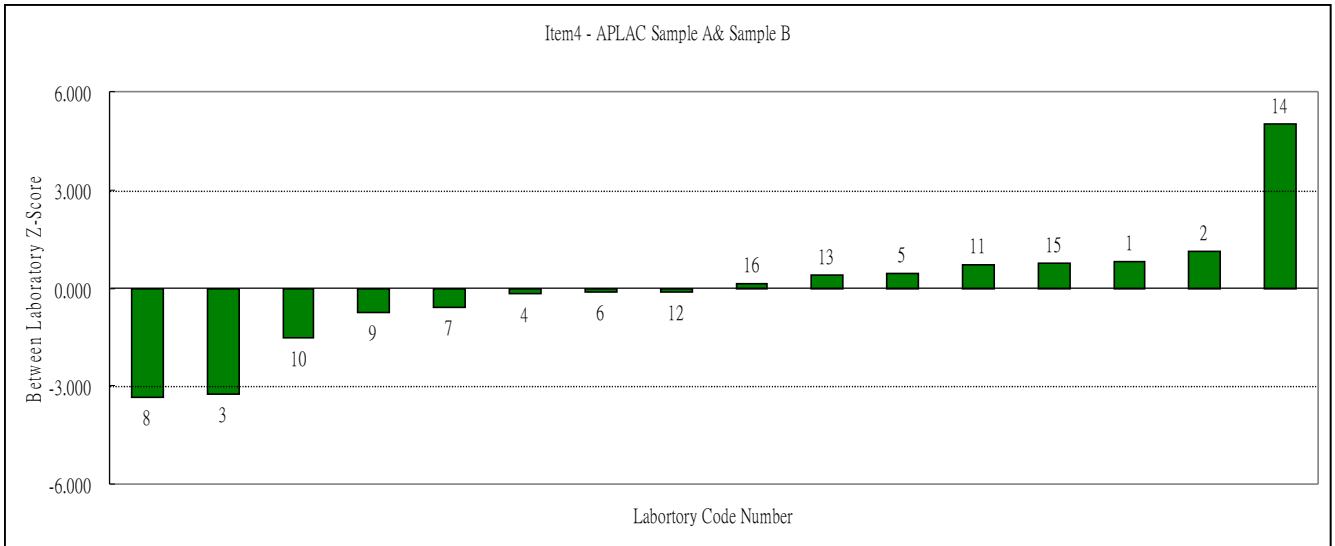

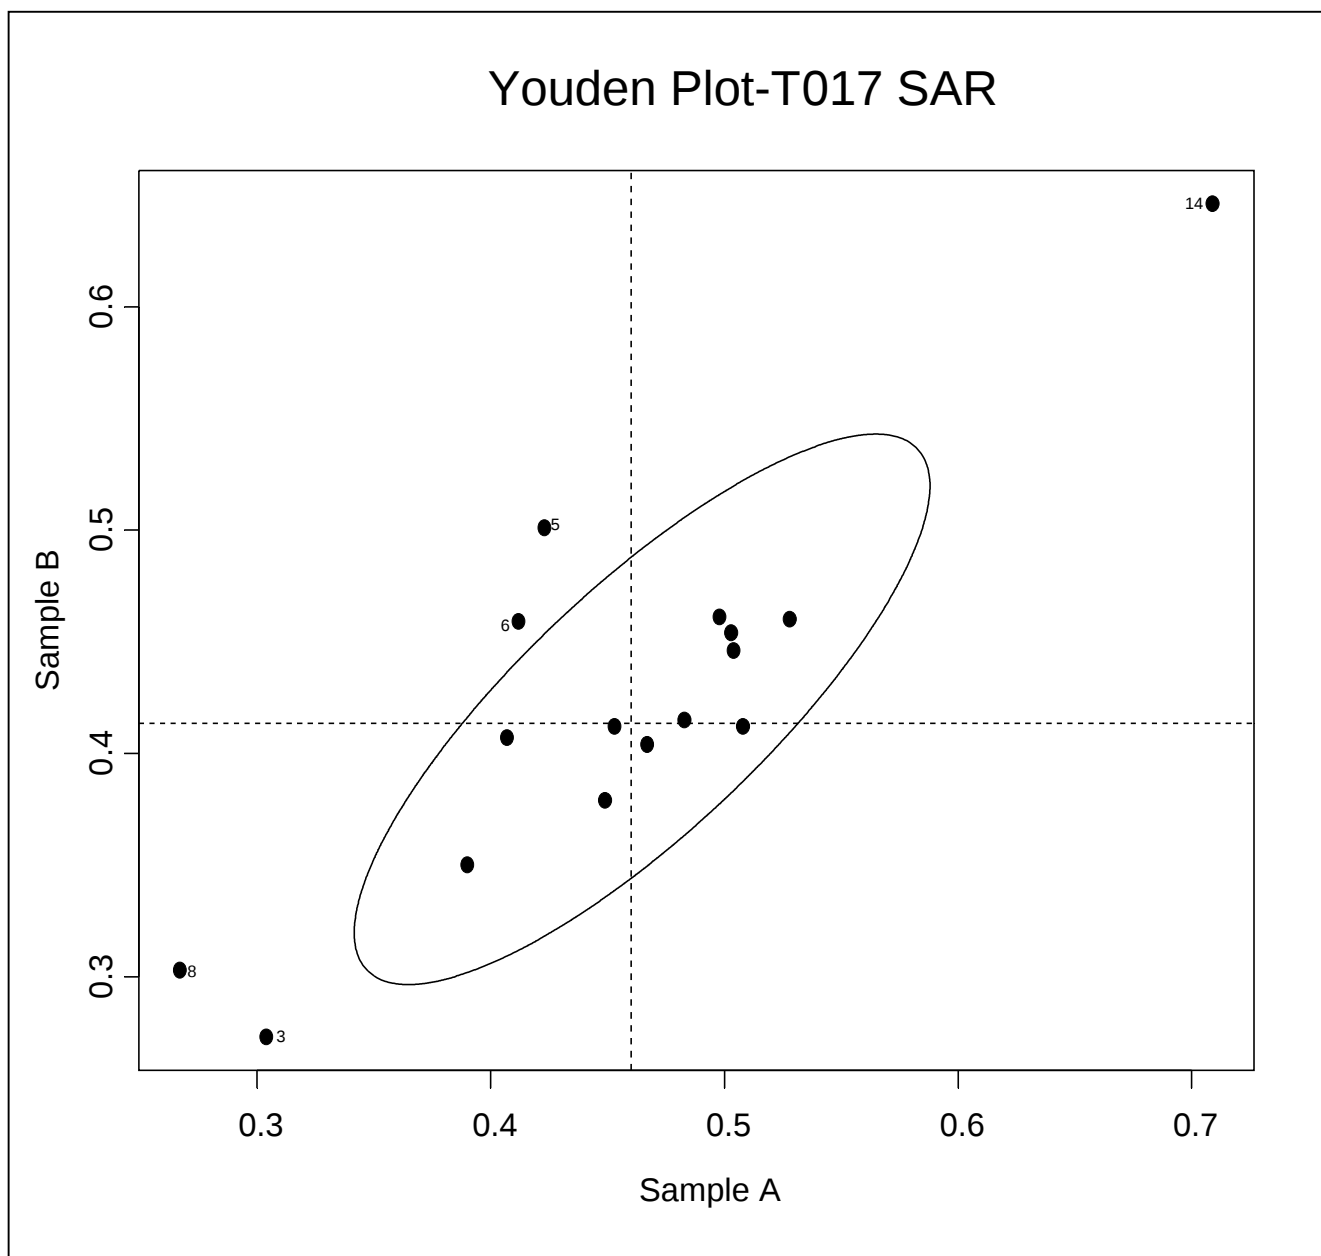

A5.1

Item 5



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
5	1710.2	512	0	30	Left Head	Cheek

Lab Code	Sample A Result	Sample B Result	Between Laboratories	Within Laboratories	Expanded uncertainty	
	SAR(mW/g)	SAR(mW/g)	Z-Score	Z-Score	Sample A	Sample B
1	0.441	0.472	9.958	-0.544	±0.84%	±0.92%
2	0.528	0.559	1.674	-0.544	±23.83%	±23.83%
3	0.241	0.273	-3.512✖	-0.495	±40.6%	±40.6%
4	0.436	0.469	2.716	-0.445	±20.6%	±20.6%
5	0.422	0.601	1.095	6.782✖	±29.1%	±29.1%
6	0.356	0.464	-0.742	3.267✖	±20.6%	±20.6%
7	0.37	0.417	-1.041	0.247	±23.7%	±23.7%
8	0.252	0.287	-3.286✖	-0.346	±22.63%	±22.63%
9	0.363	0.421	-1.068	0.792	±20.6%	±20.6%
10	0.34	0.29	-2.462	-4.554✖	±18.4%	±18.4%
11	0.464	0.484	0.416	-1.089	±27%	±27%
12	0.39	0.432	-0.724	0	±22%	±22%
13	0.43	0.472	0	0	±12.61%	±12.61%
14	0.56	0.622	2.534	0.99	±27.5%	±27.5%
15	0.434	0.497	0.262	1.039	±20.6%	±20.6%
16	0.422	0.48	0	0.792	±20.6%	±20.6%


No. of	16	16
Median	0.422	0.47
Normalized IQR	5.633	0.049
Robust CV(%)	13.35	10.595
Maximum	0.56	0.622
Minimum	0.241	0.273
Range	0.319	0.349

A5.2

Item 5 – APLAC Sample A & Sample B

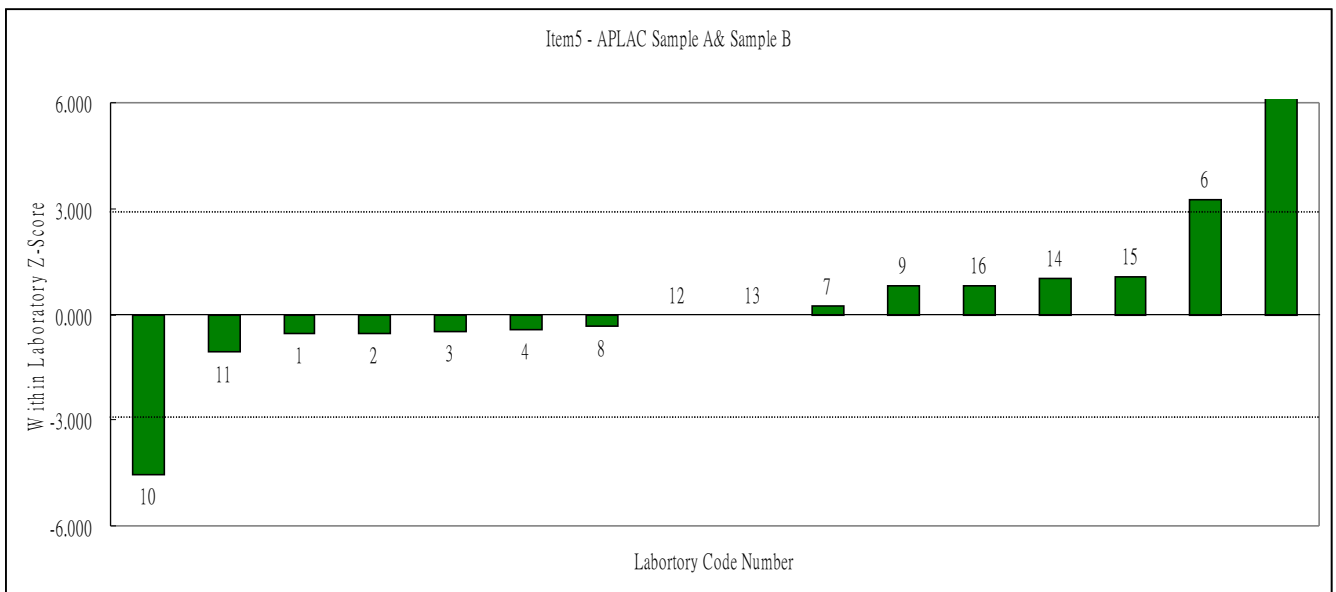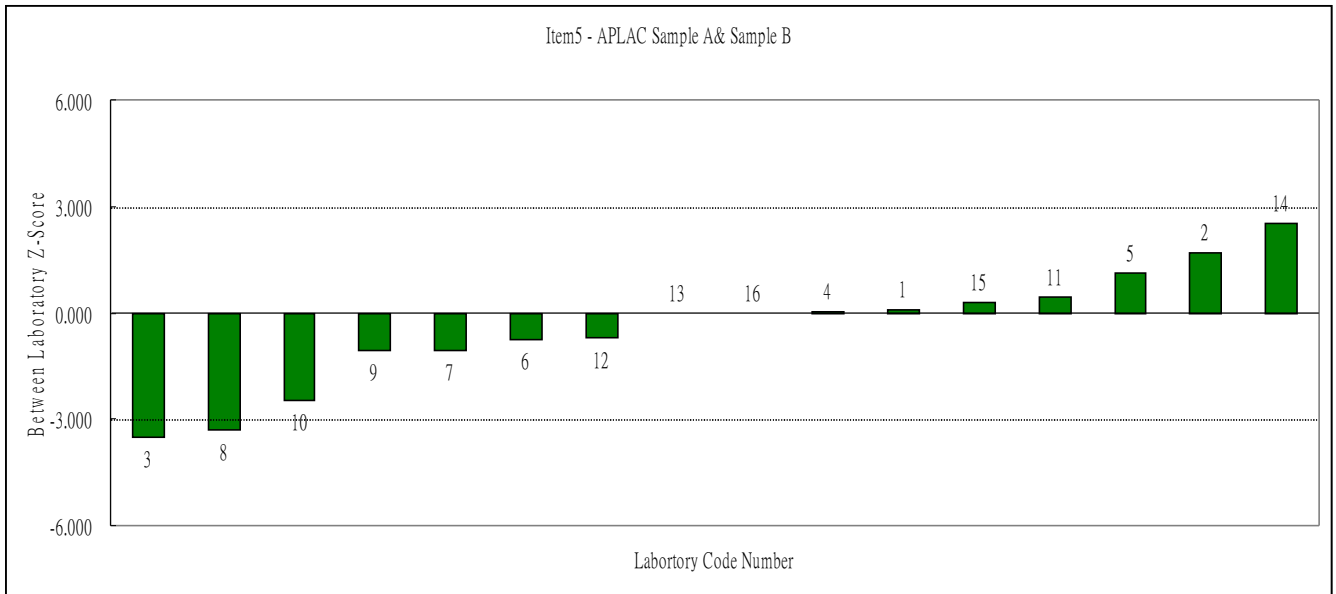

Youden Plot-T017 SAR

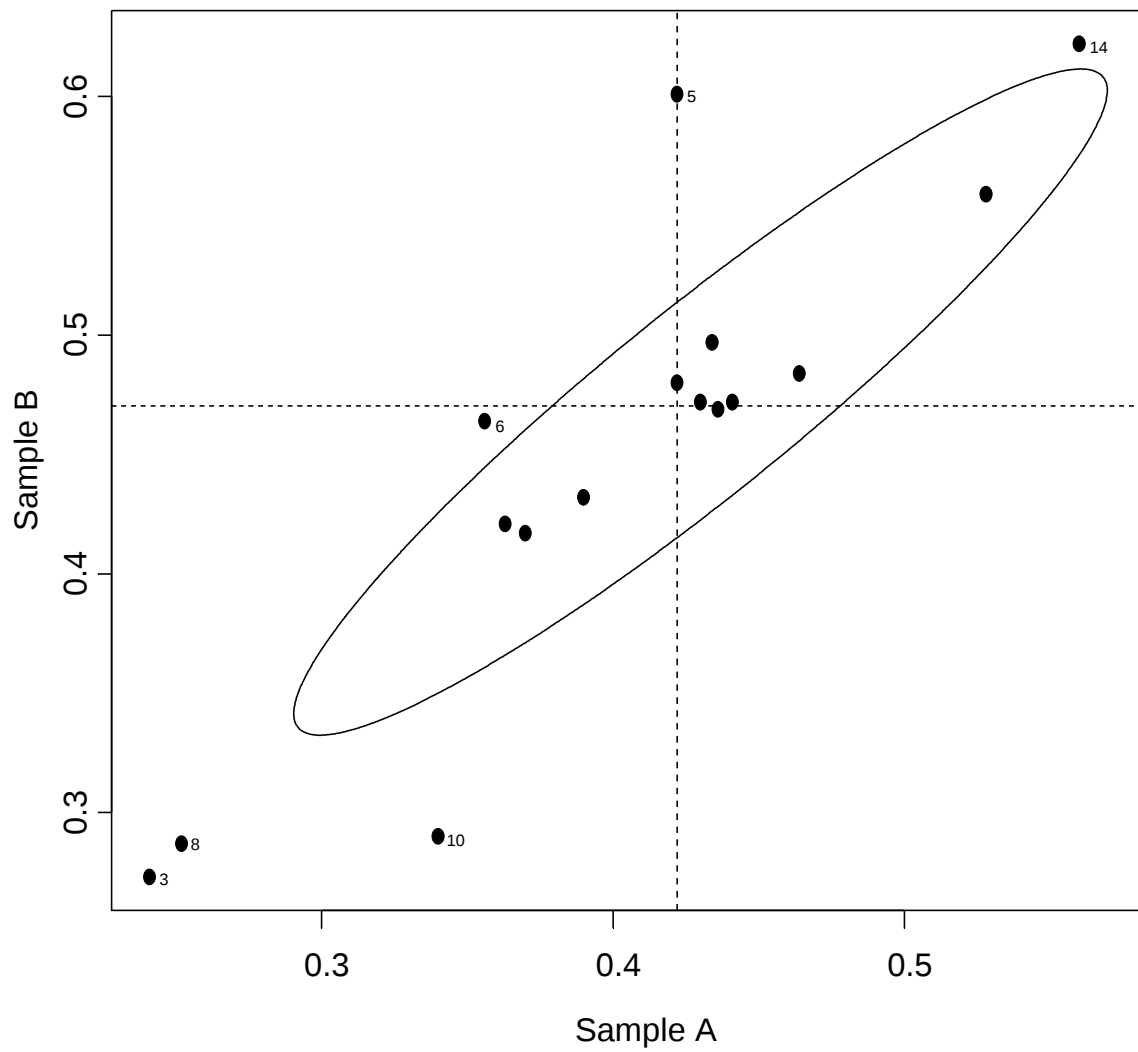

A6.1
Item 6



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
6	1710.2	512	0	30	Left Head	Tilted 15 °


Lab Code	Sample A	Sample B	Between	Within	Expanded uncertainty	
	Result	Result	Laboratories	Laboratories	Sample A	Sample B
	SAR(mW/g)	SAR(mW/g)	Z-Score	Z-Score		
1	0.337	0.363	0.298	0.321	±0.84%	±0.92%
2	0.393	0.421	2.495	0.578	±23.83%	±23.83%
3	0.191	0.189	-5.868✖	-3.276✖	±40.6%	±40.6%
4	0.332	0.355	0.048	-6.423	±20.6%	±20.6%
5	0.322	0.431	1.32	10.984✖	±29.1%	±29.1%
6	0.289	0.357	-0.741	5.717✖	N/A	N/A
7	0.302	0.328	-1.05	0.321	N/A	N/A
8	0.251	0.267	-3.208✖	-0.963	±22.63%	±22.63%
9	0.318	0.342	-0.472	6.423	±20.6%	±20.6%
10	0.33	0.27	-1.628	-10.727✖	N/A	N/A
11	0.338	0.354	0.144	-0.963	±27%	±27%
12	0.328	0.342	-0.279	-1.22	±22%	±22%
13	0.336	0.355	0.125	-0.578	±12.61%	±12.61%
14	0.421	0.483	4.230✖	4.946✖	N/A	N/A
15	0.361	0.387	1.223	0.321	N/A	N/A
16	0.333	0.349	-0.048	-0.963	±20.6%	±20.6%

No. of	16	16
Median	0.331	0.354
Normalized IQR	0.017	0.022
Robust CV(%)	5.207	6.377
Maximum	0.421	0.483
Minimum	0.191	0.189
Range	0.23	0.294

NOTE : ✖ denotes an outlier (i.e. |z-score| ≥ 3)

A6.2
Item 6 – APLAC Sample A & Sample B

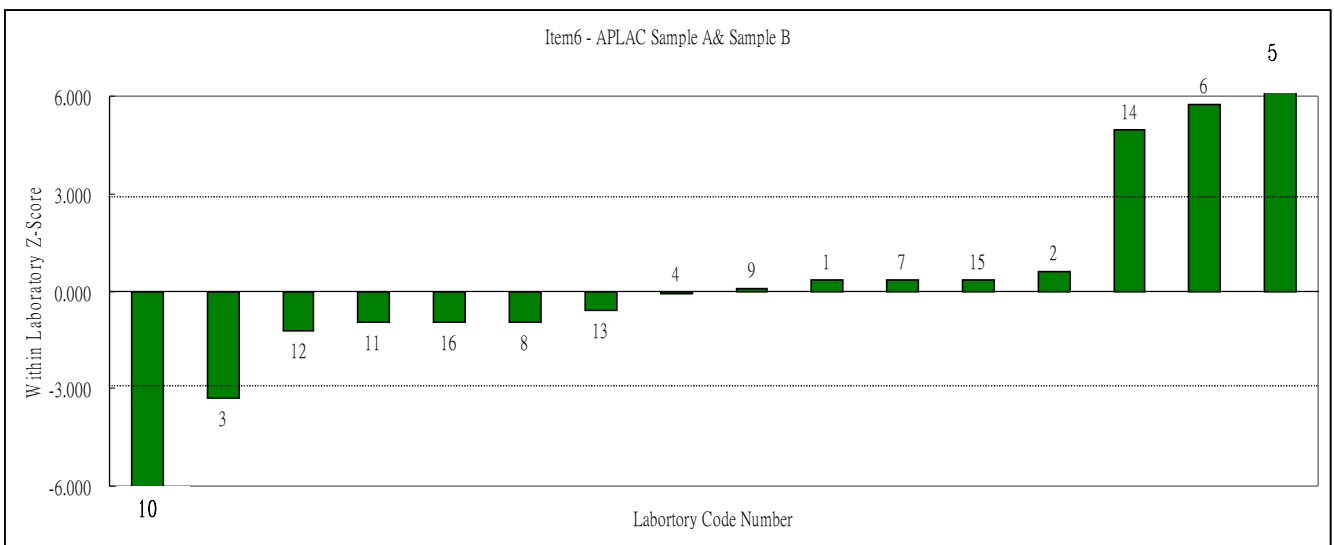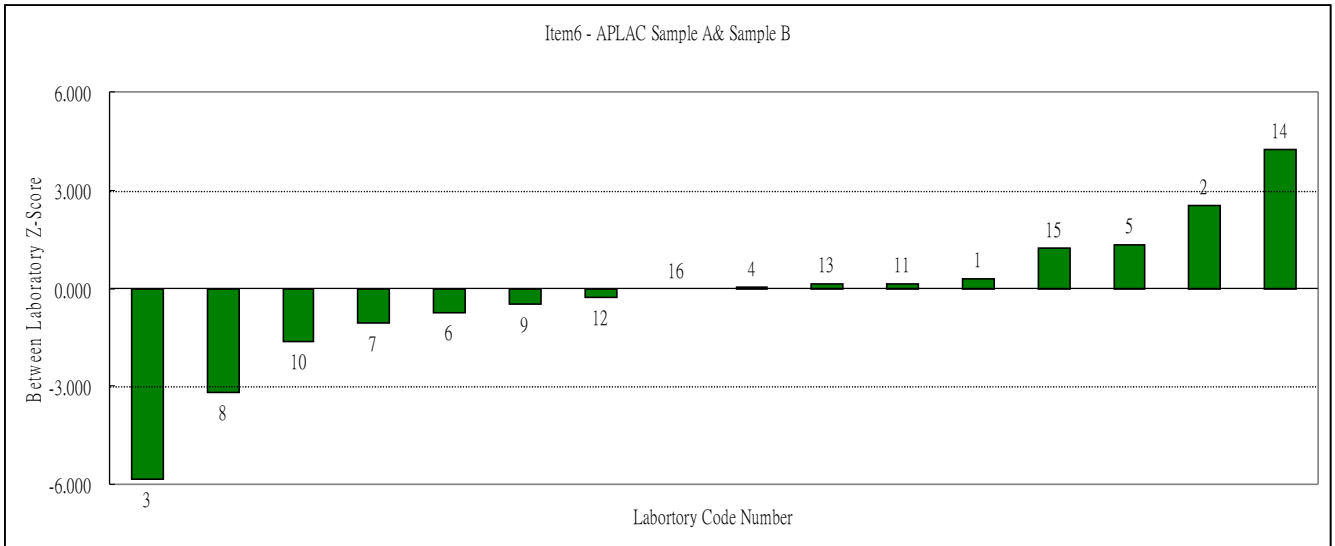

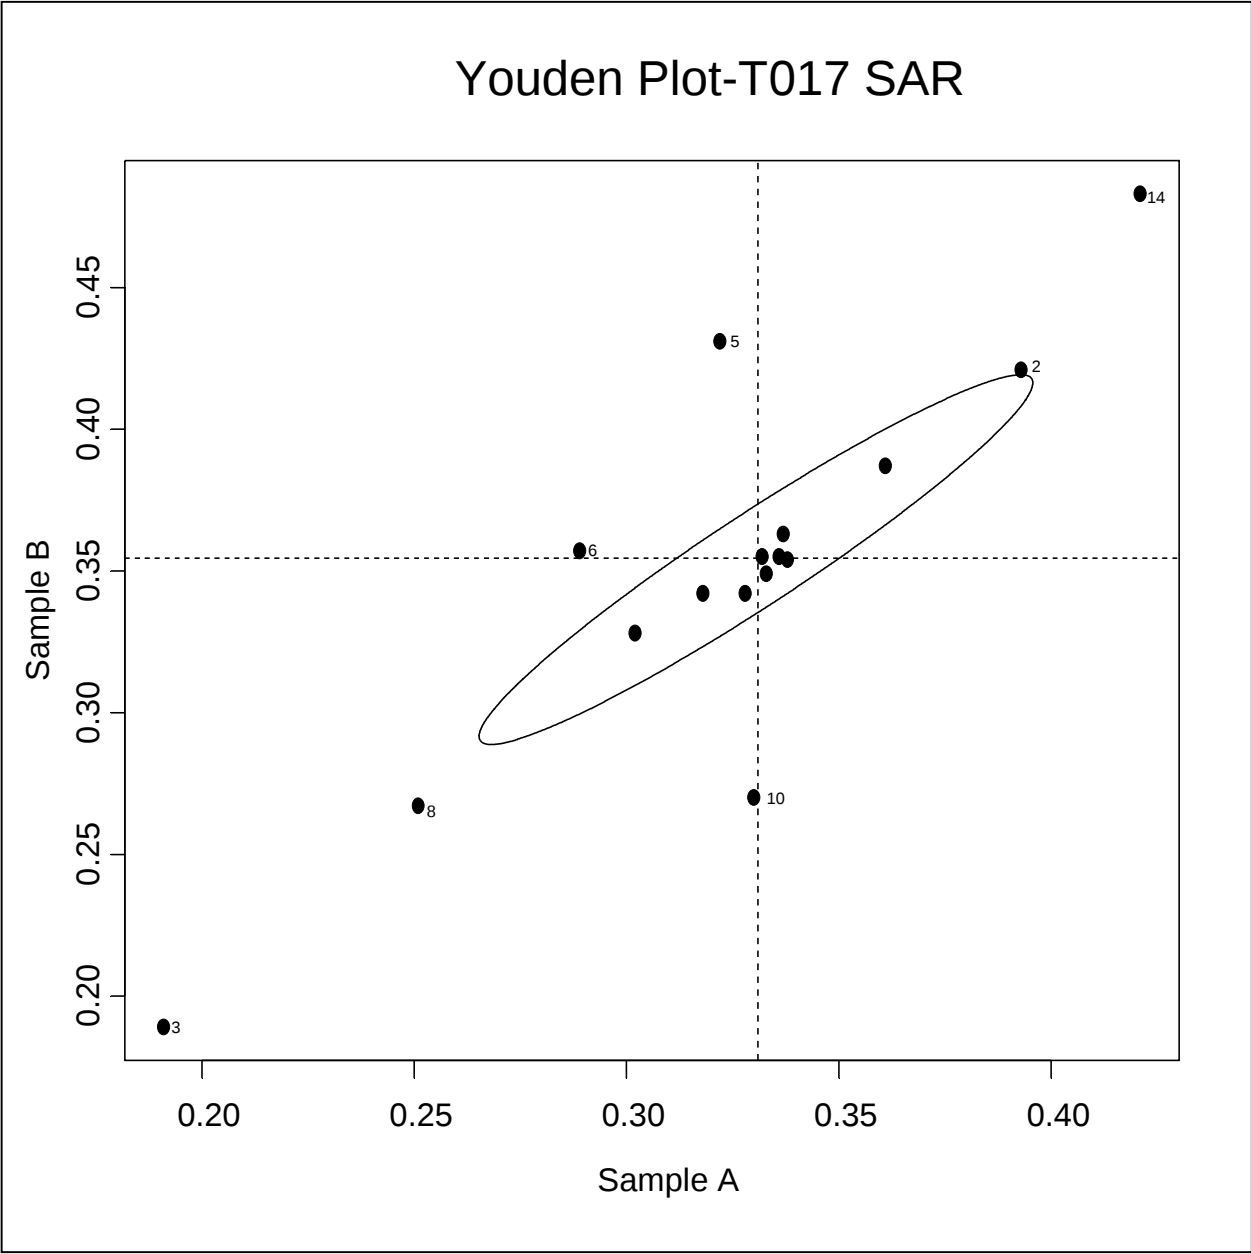

A7.1

Item 7



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
7	1710.2	512	0	30	Right Head	Cheek

Lab Code	Sample A	Sample B	Between	Within	Expanded uncertainty	
	Result SAR(mW/g)	Result SAR(mW/g)	Laboratories Z-Score	Laboratories Z-Score	Sample A	Sample B
1	0.507	0.462	0.697	-0.911	±0.84%	±0.92%
2	0.612	0.465	2.513	1.671	±23.83%	±23.83%
3	0.465	0.328	-2.26	1.418	±40.6%	±40.6%
4	0.513	0.418	5.883	0.354	±20.6%	±20.6%
5	0.401	0.48	-0.781	-4.053※	±29.1%	±29.1%
6	0.599	0.489	2.697	0.734	N/A	N/A
7	0.511	0.435	0.31	-0.126	N/A	N/A
8	0.336	0.329	-4.412※	-1.874	±22.63%	±22.63%
9	0.488	0.467	0.462	-1.519	±20.6%	±20.6%
10	0.48	0.39	-0.966	0.227	N/A	N/A
11	0.488	0.426	-0.226	-0.481	±27%	±27%
12	0.462	0.38	-1.437	2.533	±22%	±22%
13	0.519	0.405	-5.883	0.835	±12.61%	±12.61%
14	0.564	0.369	0.092	2.887	N/A	N/A
15	0.564	0.484	2.025	-2.533	N/A	N/A
16	0.499	0.424	-7.564	-0.151	±20.6%	±20.6%


No. of	16	16
Median	0.503	0.425
Normalized IQR	0.04	0.057
Robust CV(%)	7.958	13.605
Maximum	0.612	0.489
Minimum	0.336	0.328
Range	0.276	0.161

NOTE : ※ denotes an outlier (i.e. lz-scorel ≥ 3)

A7.2
Item 7 – APLAC Sample A & Sample B

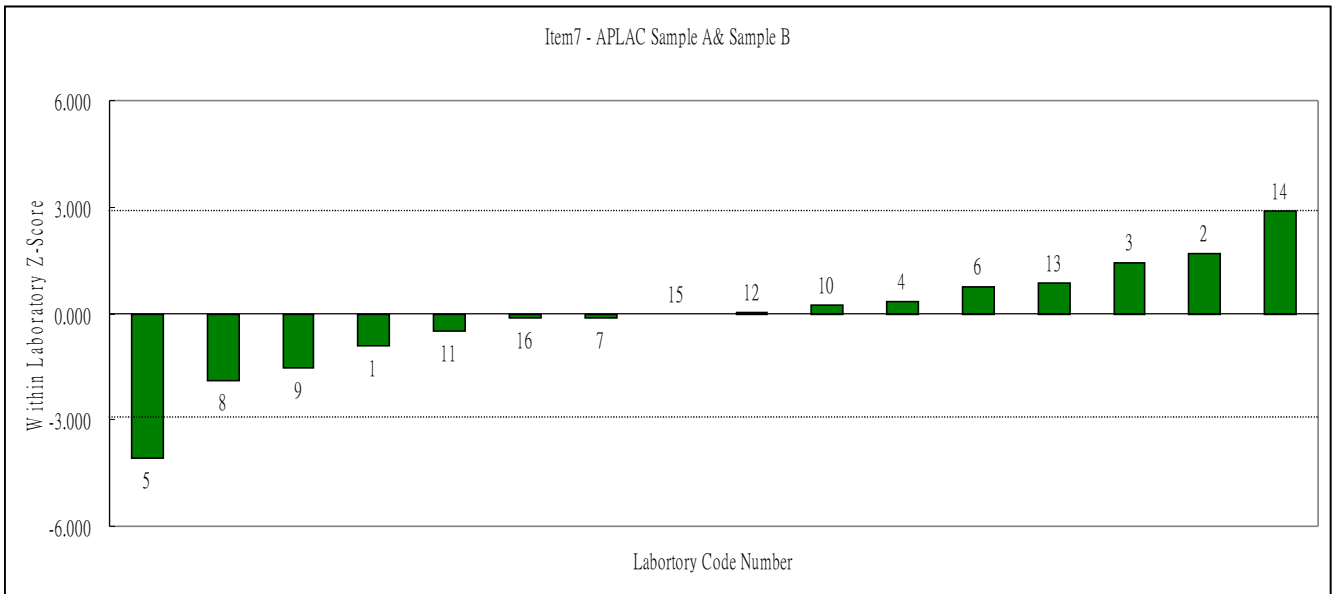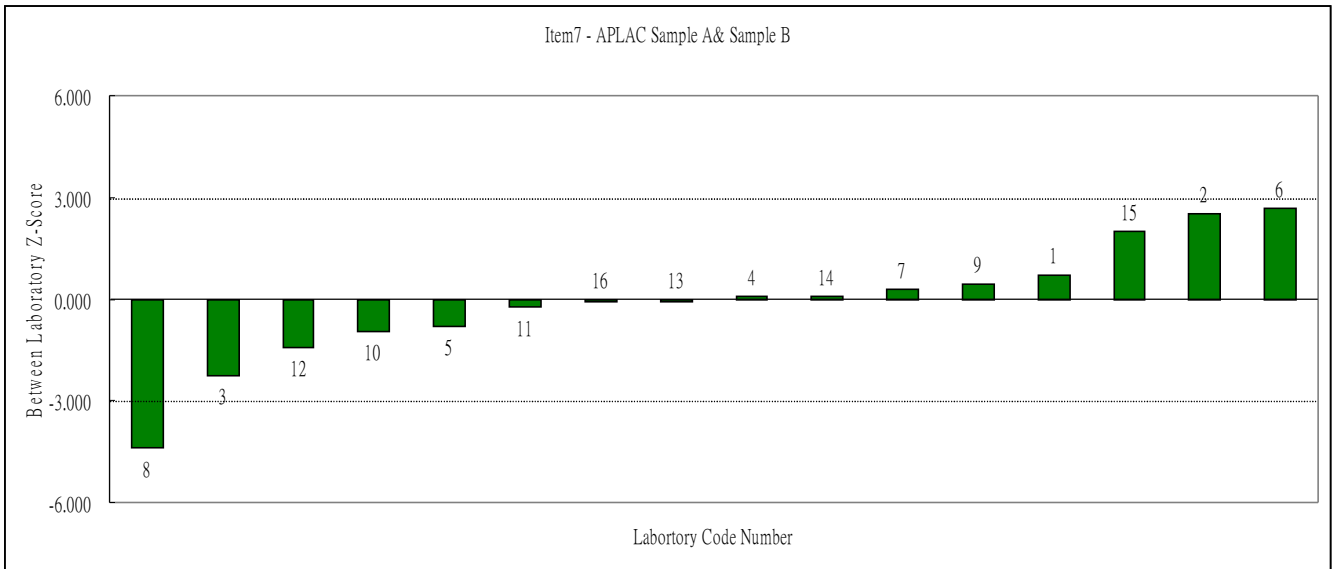

Youden Plot-T017 SAR

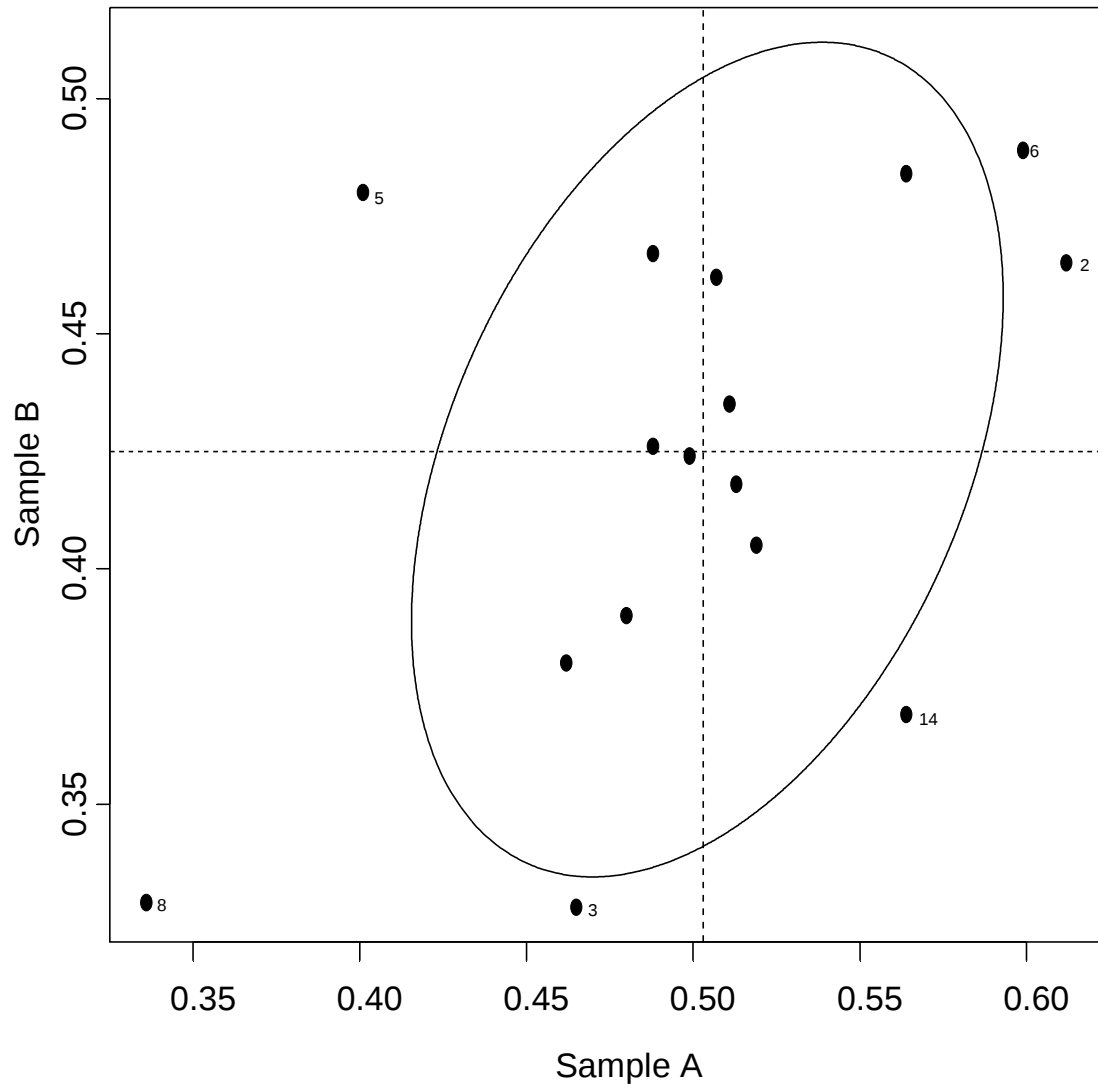

A8.1**Item 8**



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
8	1747.8	700	0	30	Right Head	Cheek


Lab Code	Sample A Result	Sample B Result	Between Laboratories	Within Laboratories	Expanded uncertainty	
	SAR(mW/g)	SAR(mW/g)	Z-Score	Z-Score	Sample A	Sample B
1	0.365	0.414	-0.656	0.854	±0.84%	±0.92%
2	0.537	0.528	2.697	-0.259	±23.83%	±23.83%
3	0.415	0.351	-0.809	-1.315	±40.6%	±40.6%
4	0.417	0.437	0.222	0.297	±20.6%	±20.6%
5	0.344	0.511	0.234	3.120※	±29.1%	±29.1%
6	0.551	0.502	2.557	-1.027	N/A	N/A
7	0.401	0.419	-0.175	0.259	N/A	N/A
8	0.267	0.3	-3.143※	0.547	±22.63%	±22.63%
9	0.383	0.422	-0.351	0.662	±20.6%	±20.6%
10	0.4	0.34	-1.114	-1.238	N/A	N/A
11	0.454	0.451	0.821	-0.144	±27%	±27%
12	0.363	0.364	-1.266	-6.72	±22%	±22%
13	0.459	0.427	0.598	-0.7	±12.61%	±12.61%
14	0.486	0.346	-3.519	-2.774	N/A	N/A
15	0.463	0.5	1.501	0.624	N/A	N/A
16	0.415	0.423	3.519	6.72	±20.6%	±20.6%

No. of	16	16
Median	0.415	0.422
Normalized IQR	0.06	0.075
Robust CV(%)	14.558	17.984
Maximum	0.551	0.528
Minimum	0.267	0.3
Range	0.284	0.228

NOTE : ※ denotes an outlier (i.e. |z-score| ≥ 3)

A8.2
Item 8 – APLAC Sample A & Sample B

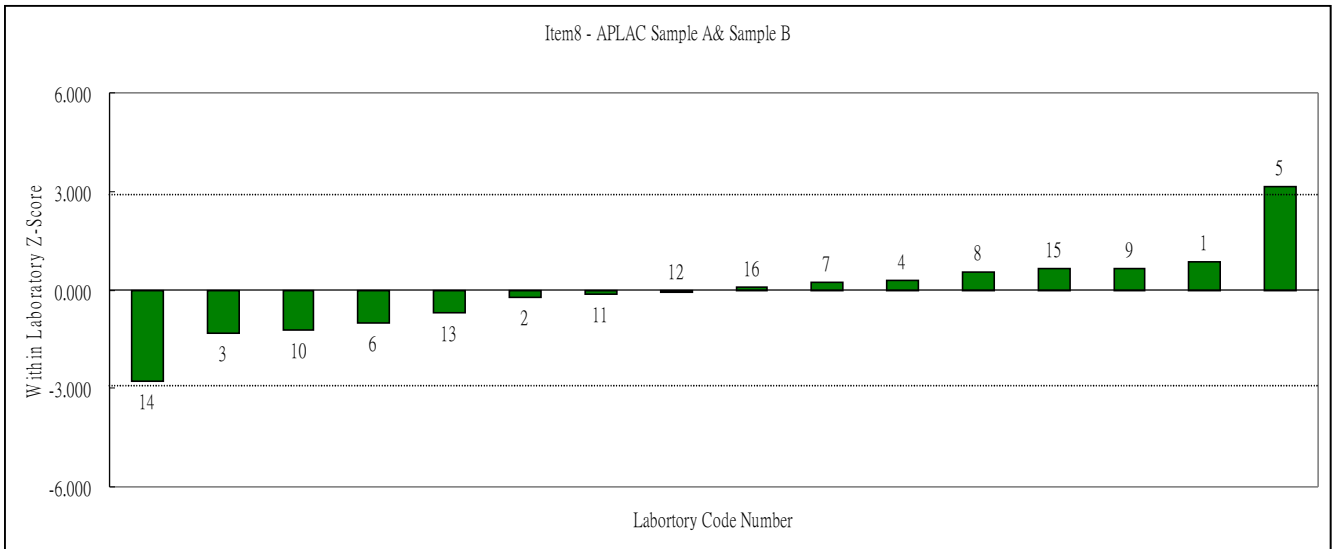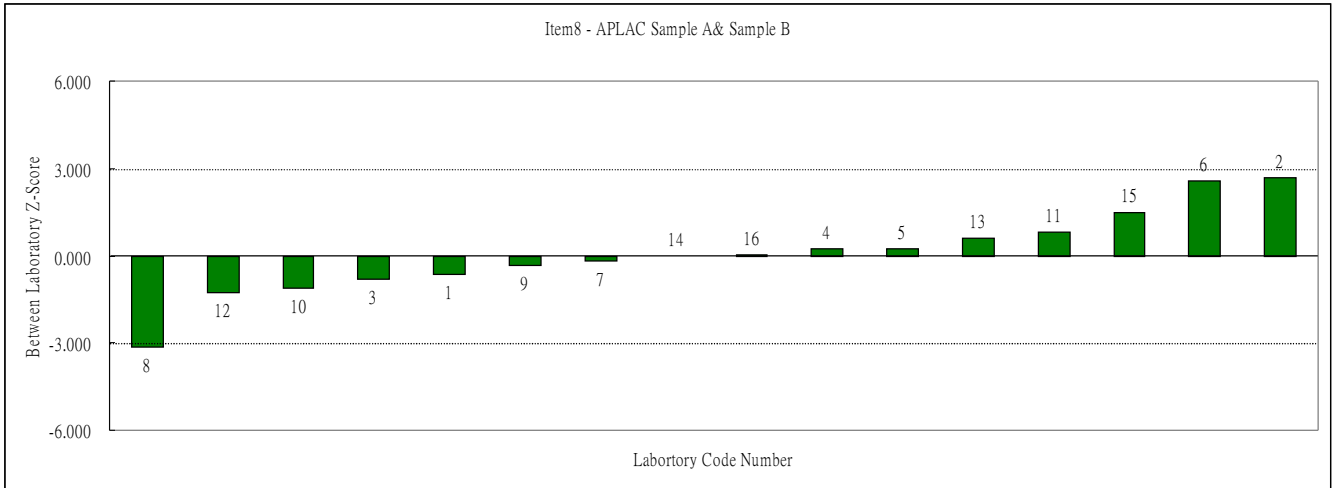

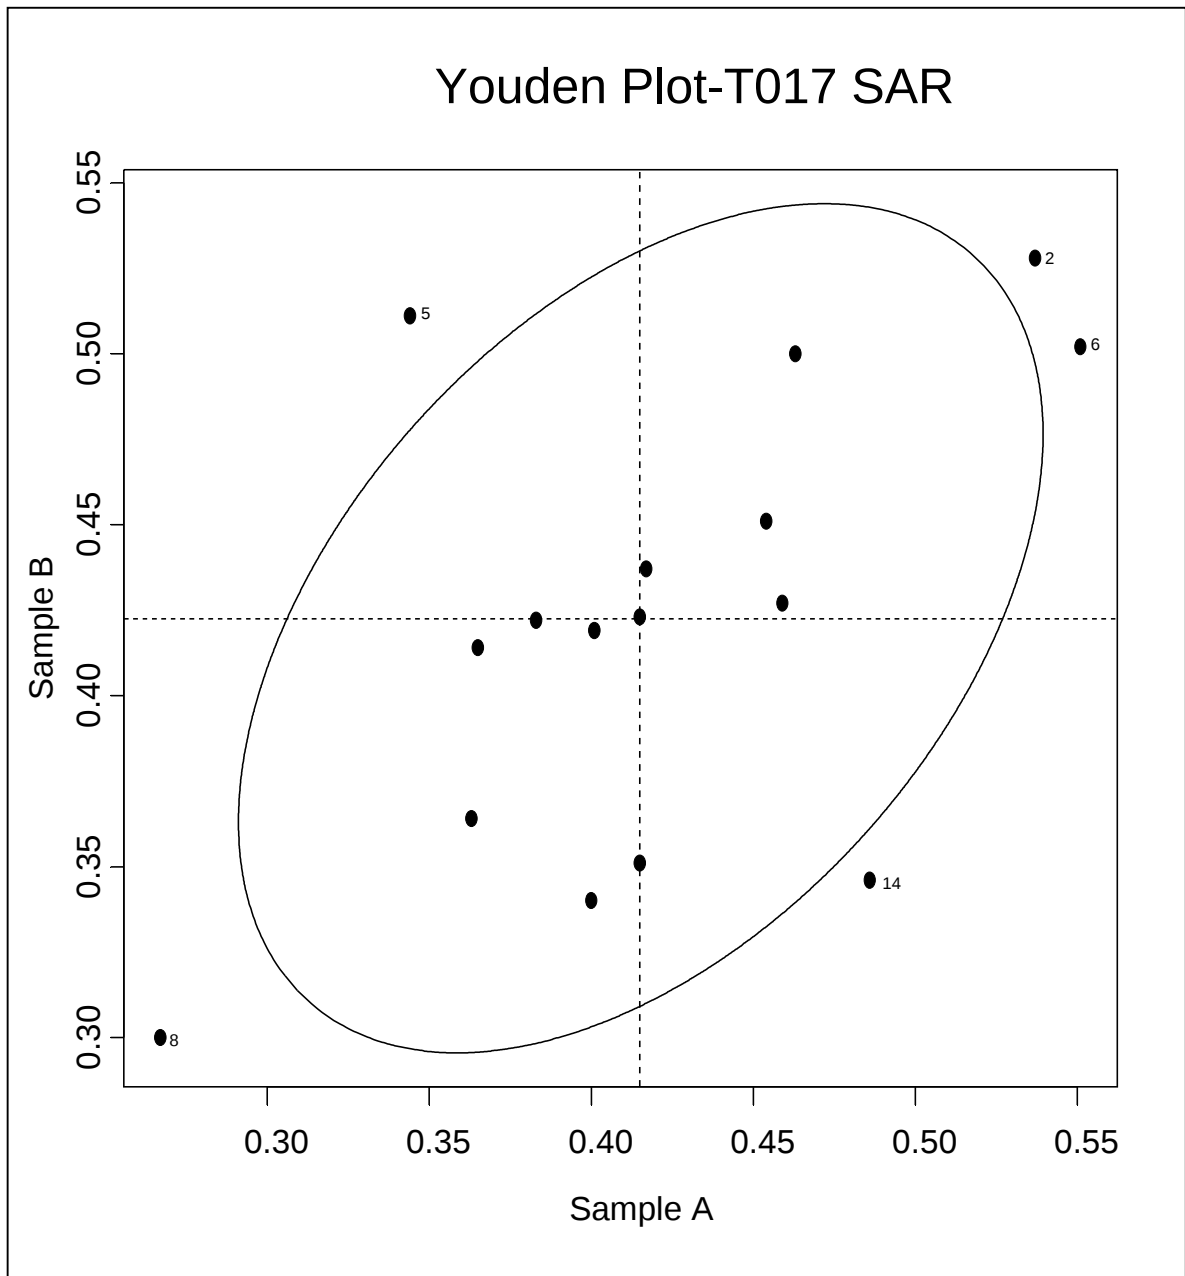

A9.1

Item 9



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
9	1784.8	885	0	30	Right Head	Cheek

Lab Code	Sample A Result	Sample B Result	Between Laboratories	Within Laboratories	Expanded uncertainty	
	SAR(mW/g)	SAR(mW/g)	Z-Score	Z-Score	Sample A	Sample B
1	0.273	0.316	-1.006	-0.983	±0.84%	±0.92%
2	0.393	0.354	2.174	0.891	±23.83%	±23.83%
3	0.335	0.268	-0.724	1.531	±40.6%	±40.6%
4	0.313	0.321	-0.1	-0.182	±20.6%	±20.6%
5	0.291	0.378	0.604	-1.989	±29.1%	±29.1%
6	0.408	0.39	3.201※	0.411	N/A	N/A
7	0.311	0.327	-2.013	-0.365	N/A	N/A
8	0.209	0.24	-3.825※	-0.708	±22.63%	±22.63%
9	0.328	0.326	0.302	0.045	±20.6%	±20.6%
10	0.39	0.34	1.832	1.143	N/A	N/A
11	0.343	0.314	0.362	0.663	±27%	±27%
12	0.275	0.281	-1.671	-0.137	±22%	±22%
13	0.331	0.291	-0.342	0.914	±12.61%	±12.61%
14	0.374	0.266	2.013	2.469	N/A	N/A
15	0.359	0.394	2.295	-0.8	N/A	N/A
16	0.316	0.318	-0.1	-0.045	±20.6%	±20.6%


No. of	16	16
Median	0.329	0.319
Normalized IQR	0.042	0.04
Robust CV(%)	12.767	12.761
Maximum	0.408	0.394
Minimum	0.209	0.24
Range	0.199	0.154

NOTE : ※ denotes an outlier (i.e. |z-score| ≥ 3)

A9.2
Item 9 – APLAC Sample A & Sample B

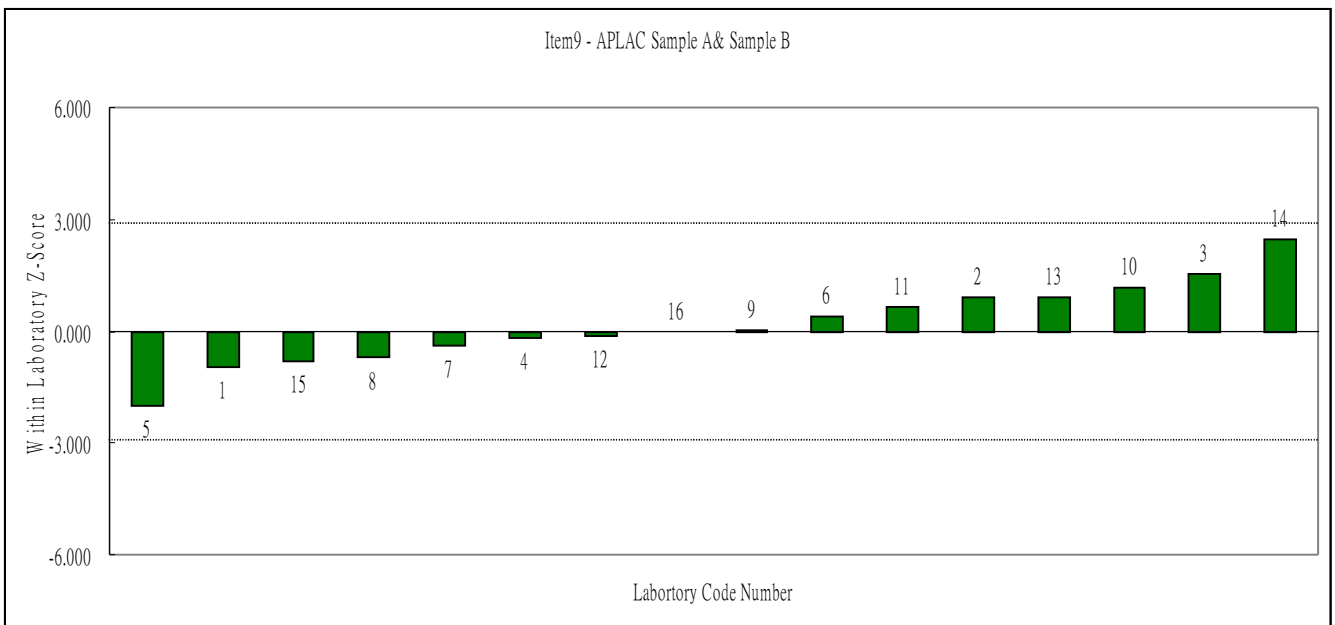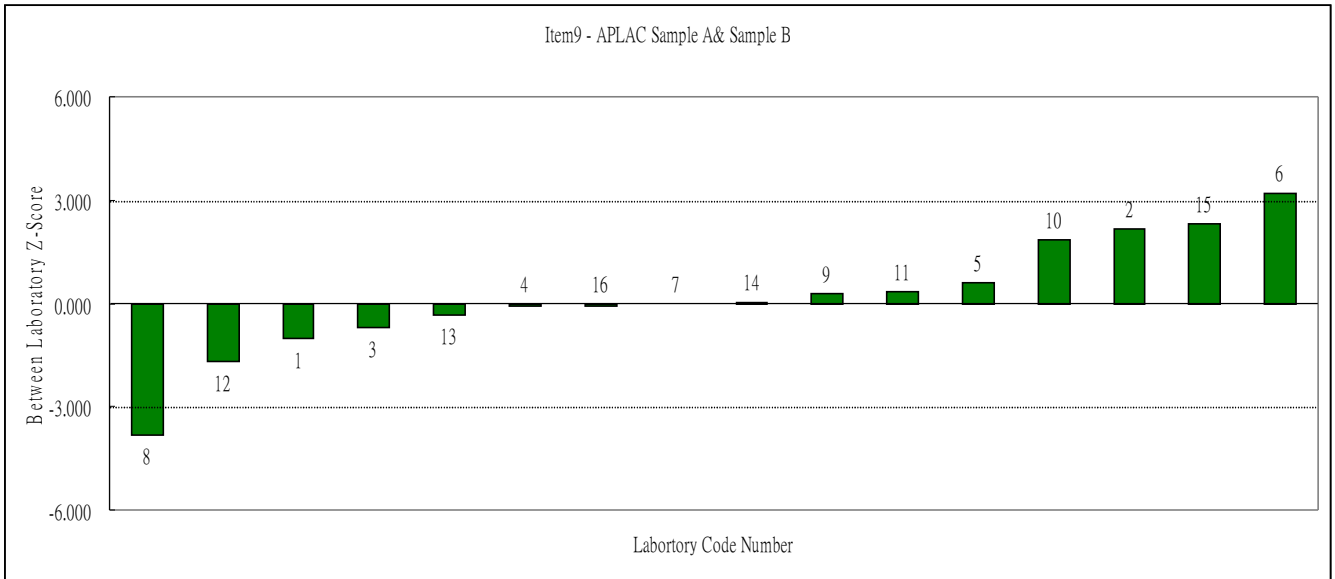

Youden Plot-T017 SAR

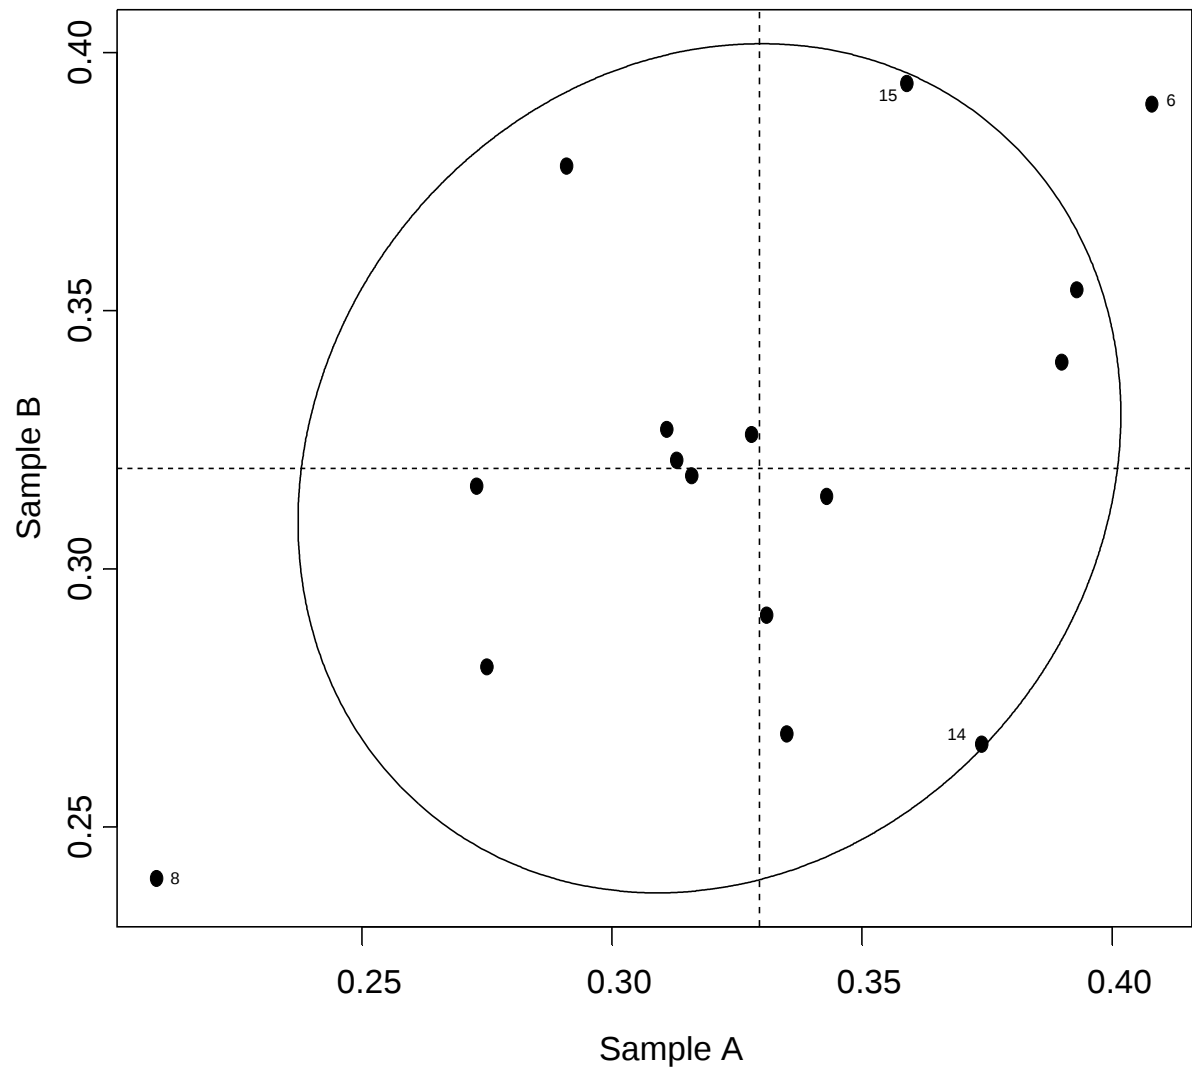

A10.1

Item 10



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
10	1710.2	512	0	30	Right Head	Tilted 15 °

Lab Code	Sample A Result	Sample B Result	Between Laboratories	Within Laboratories	Expanded uncertainty	
	SAR(mW/g)	SAR(mW/g)	Z-Score	Z-Score	Sample A	Sample B
1	0.344	0.305	-0.211	0.603	±0.84%	±0.92%
2	0.412	0.377	1.586	0.319	±23.83%	±23.83%
3	0.304	0.273	-1.136	3.549	±40.6%	±40.6%
4	0.35	0.318	3.211	0.106	±20.6%	±20.6%
5	0.311	0.36	7.066	-5.644※	±29.1%	±29.1%
6	0.317	0.303	-0.584	-1.171	N/A	N/A
7	0.323	0.3	-0.546	-0.532	N/A	N/A
8	0.231	0.271	-2.1	-5.005※	±22.63%	±22.63%
9	0.319	0.293	-0.687	-0.319	±20.6%	±20.6%
10	0.32	0.29	-0.713	-3.549	N/A	N/A
11	0.395	0.327	0.725	2.662	±27%	±27%
12	0.384	0.342	0.777	0.816	±22%	±22%
13	0.33	0.368	0.417	-4.863※	±12.61%	±12.61%
14	0.43	0.301	0.841	6.993※	N/A	N/A
15	0.426	0.372	1.702	1.668	N/A	N/A
16	0.343	0.32	-3.211	-0.532	±20.6%	±20.6%


No. of	16	16
Median	0.336	0.311
Normalized IQR	0.05	0.035
Robust CV(%)	15.035	11.482
Maximum	0.43	0.377
Minimum	0.231	0.271
Range	0.199	0.106

NOTE : ※ denotes an outlier (i.e. |z-score| ≥ 3)

A10.2
Item 10 – APLAC Sample A & Sample B

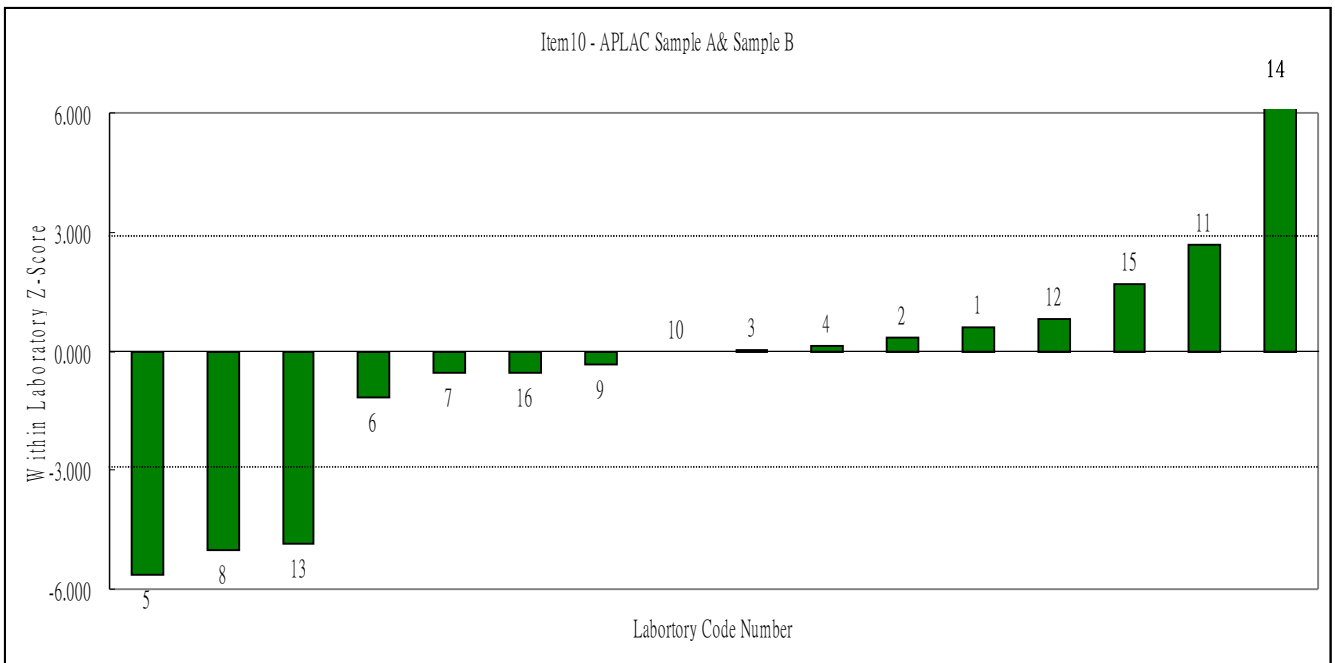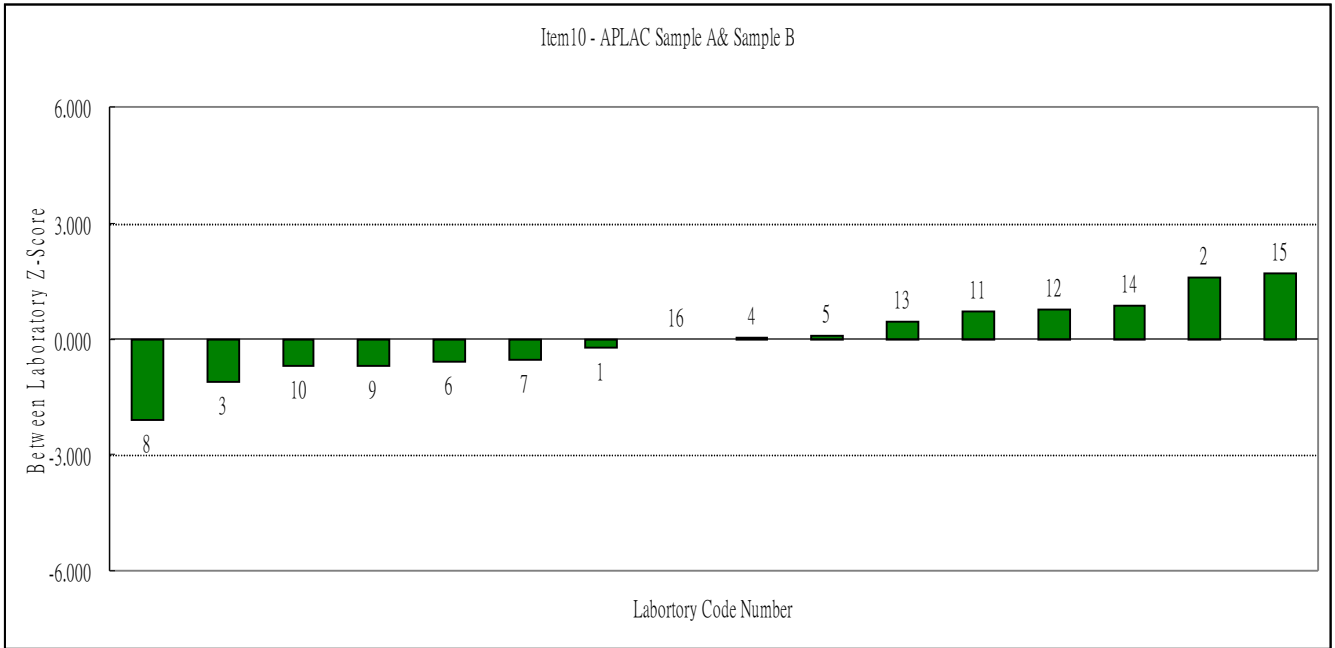

Youden Plot-T017 SAR

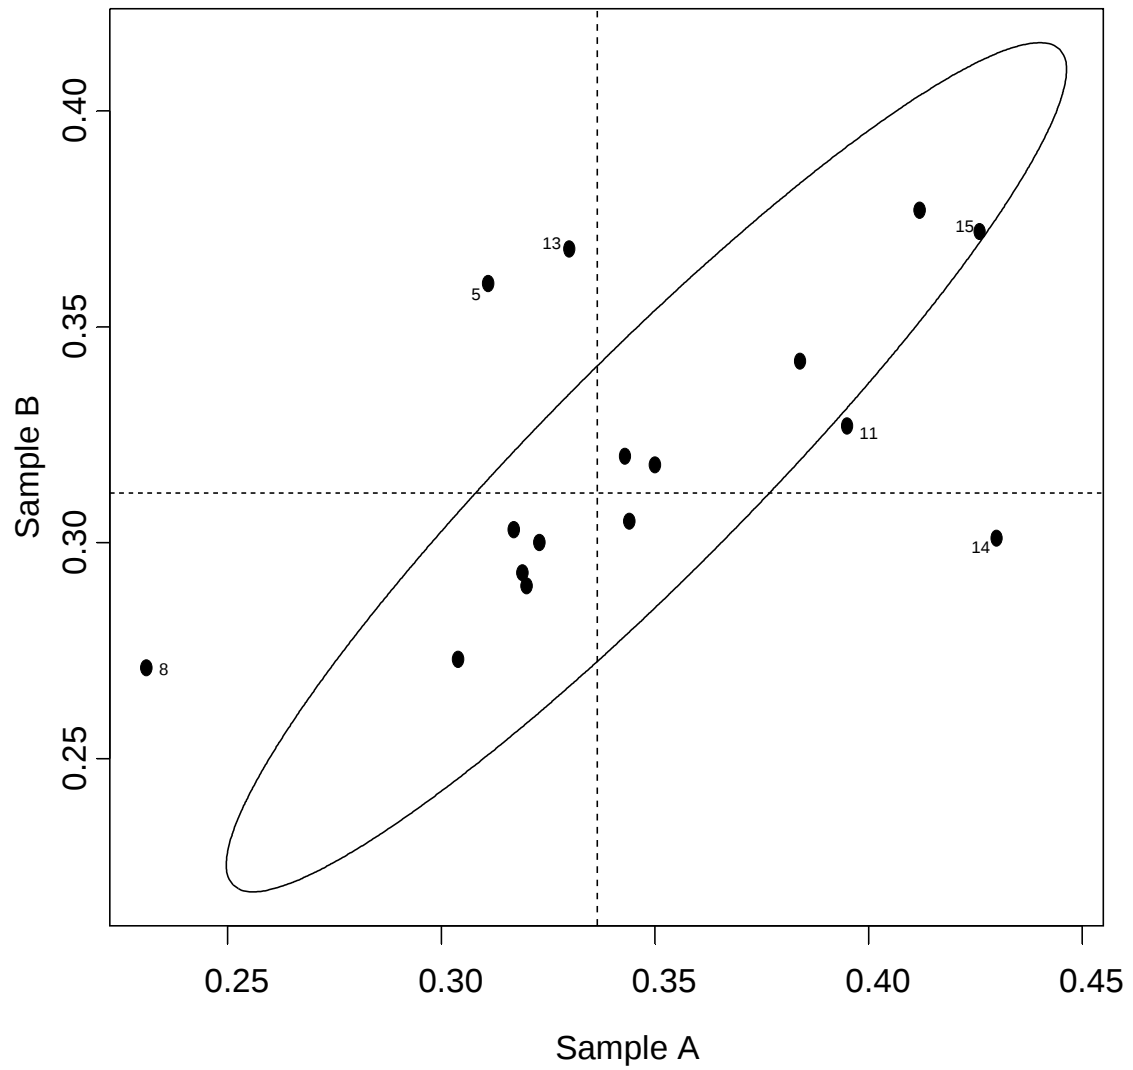

A11.1

Item11



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
11	1747.8	700	0	30	Right Head	Tilted 15 °

Lab Code	Sample A Result	Sample B Result	Between Laboratories	Within Laboratories	Expanded uncertainty	
	SAR(mW/g)	SAR(mW/g)	Z-Score	Z-Score	Sample A	Sample B
1	0.308	0.331	0.111	-0.417	±0.84%	±0.92%
2	0.396	0.471	2.236	1.252	±23.83%	±23.83%
3	0.241	0.273	-1.053	-0.128	±40.6%	±40.6%
4	0.306	0.335	0.13	-0.224	±20.6%	±20.6%
5	0.324	0.395	0.857	1.124	±29.1%	±29.1%
6	0.285	0.325	-0.158	0.128	N/A	N/A
7	0.284	0.331	-0.111	0.353	N/A	N/A
8	0.191	0.287	-1.388	1.927	±22.63%	±22.63%
9	0.267	0.285	-0.698	-0.578	±20.6%	±20.6%
10	0.26	0.27	-0.903	-0.835	N/A	N/A
11	0.372	0.392	1.276	-0.513	±27%	±27%
12	0.31	0.369	0.484	0.738	±22%	±22%
13	0.314	0.449	1.267	3.179※	±12.61%	±12.61%
14	0.289	0.295	-0.4	-0.963	N/A	N/A
15	0.353	0.373	0.922	-0.513	N/A	N/A
16	0.284	0.328	-0.139	0.256	±20.6%	±20.6%


No. of	16	16
Median	0.297	0.331
Normalized IQR	0.027	0.062
Robust CV(%)	9.157	18.98
Maximum	0.396	0.471
Minimum	0.191	0.27
Range	0.205	0.201

NOTE : ※ denotes an outlier (i.e. |z-score| ≥ 3)

A11.2
Item 11 – APLAC Sample A & Sample B

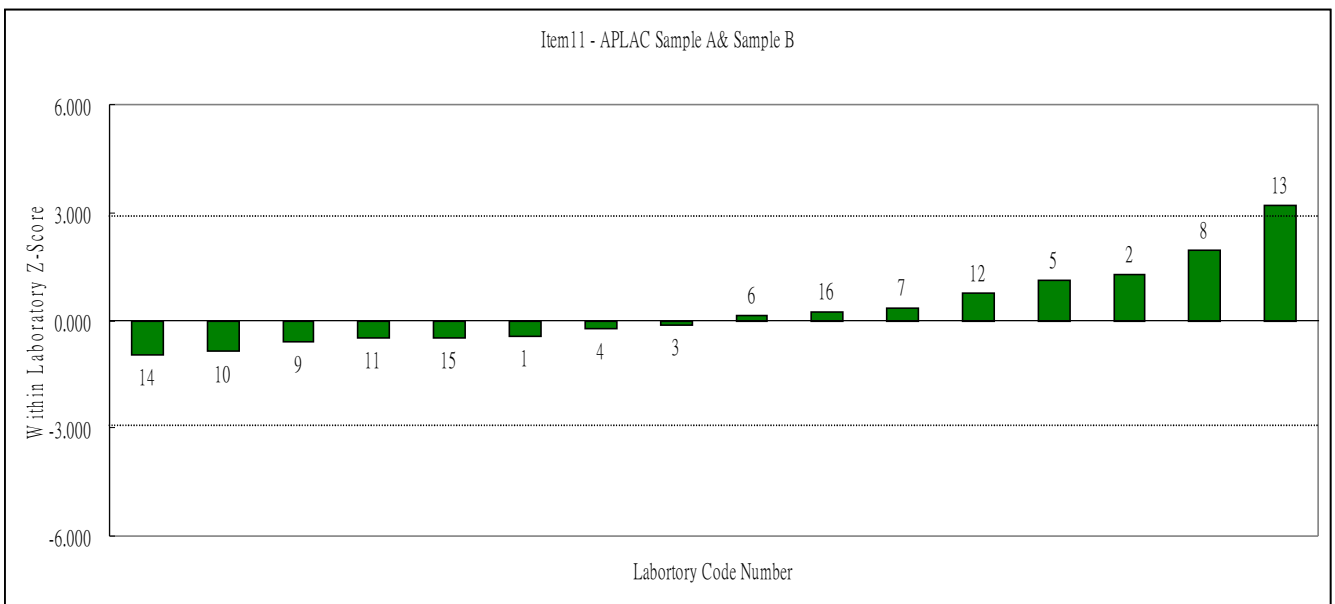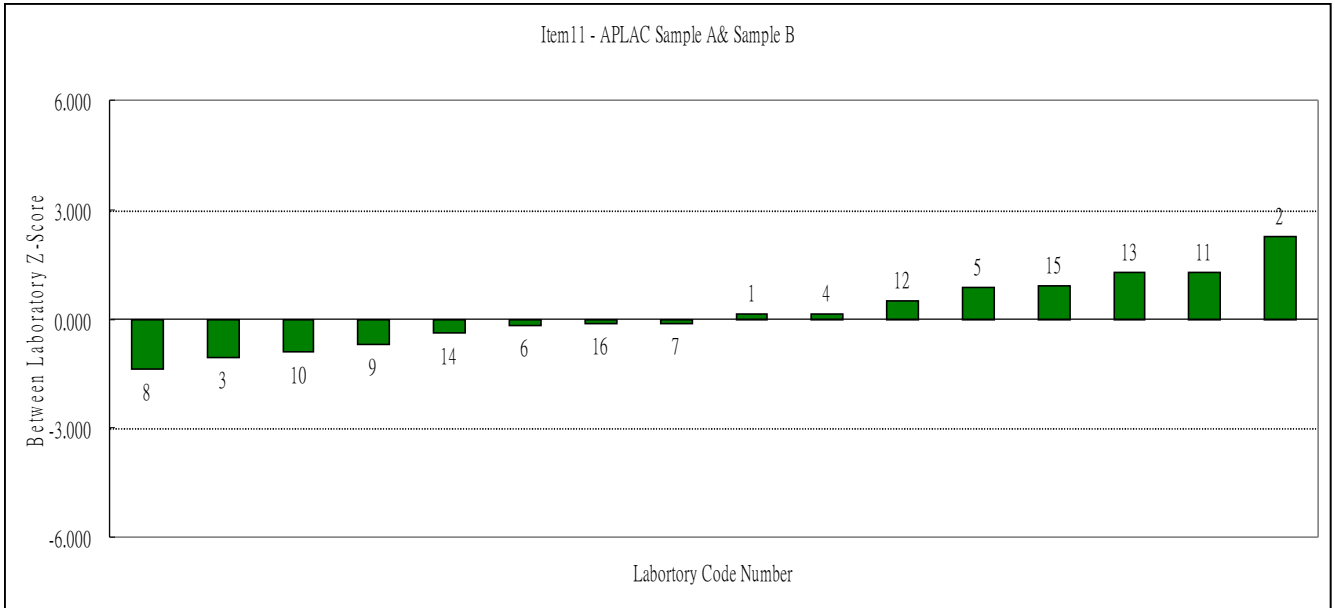

Youden Plot-T017 SAR

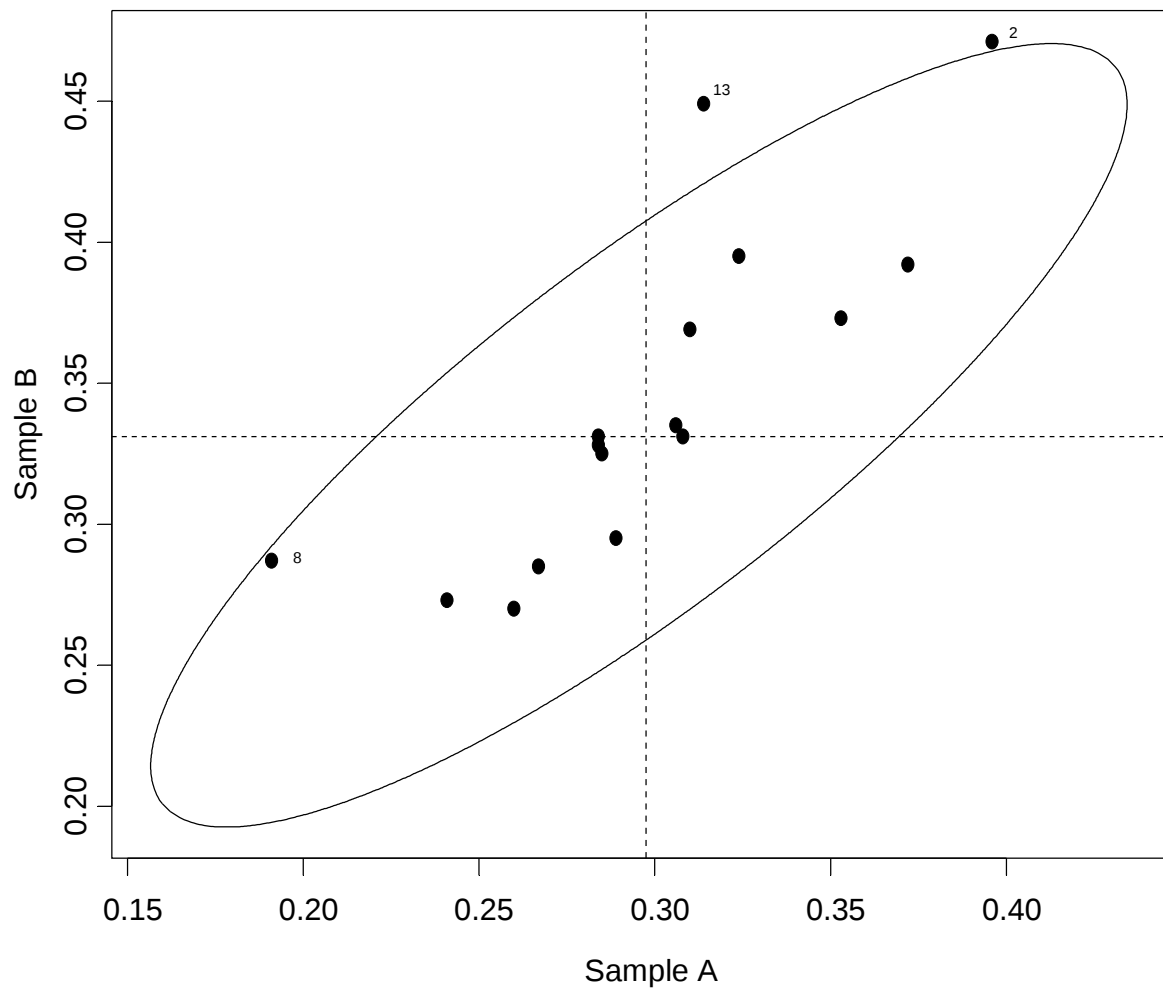

A12.1

Item 12



Item	Test Frequency		PCL	Max. Output Power (dBm)	Phantom position	Phone Position
	Frequency	Channel				
	(MHz)					
12	1784.8	885	0	30	Right Head	Tilted 15°


Lab Code	Sample A Result	Sample B Result	Between Laboratories	Within Laboratories	Expanded uncertainty	
	SAR(mW/g)	SAR(mW/g)	Z-Score	Z-Score	Sample A	Sample B
1	0.24	0.258	-0.124	-0.511	±0.84%	±0.92%
2	0.302	0.346	2.373	0.965	±23.83%	±23.83%
3	0.191	0.189	-2.09	-1.647	±40.6%	±40.6%
4	0.246	0.266	0.108	-0.397	±20.6%	±20.6%
5	0.231	0.318	0.724	3.407※	±29.1%	±29.1%
6	0.225	0.266	-0.241	0.795	N/A	N/A
7	0.233	0.268	-7.494	0.454	N/A	N/A
8	0.195	0.231	-1.324	0.511	±22.63%	±22.63%
9	0.22	0.236	-0.824	-0.624	±20.6%	±20.6%
10	0.25	0.26	7.494	-0.965	N/A	N/A
11	0.281	0.312	1.457	0.227	±27%	±27%
12	0.268	0.291	0.89	-0.227	±22%	±22%
13	0.254	0.333	1.357	2.953	±12.61%	±12.61%
14	0.209	0.21	-1.44	-1.476	N/A	N/A
15	0.278	0.298	1.174	-0.397	N/A	N/A
16	0.229	0.271	-0.091	0.851	±20.6%	±20.6%

No. of	16	16
Median	0.236	0.267
Normalized IQR	0.025	0.036
Robust CV(%)	10.578	13.604
Maximum	0.302	0.346
Minimum	0.191	0.189
Range	0.111	0.157

NOTE : ※ denotes an outlier (i.e. |z-score| ≥ 3)

A12.2
Item 12 – APLAC Sample A & Sample B

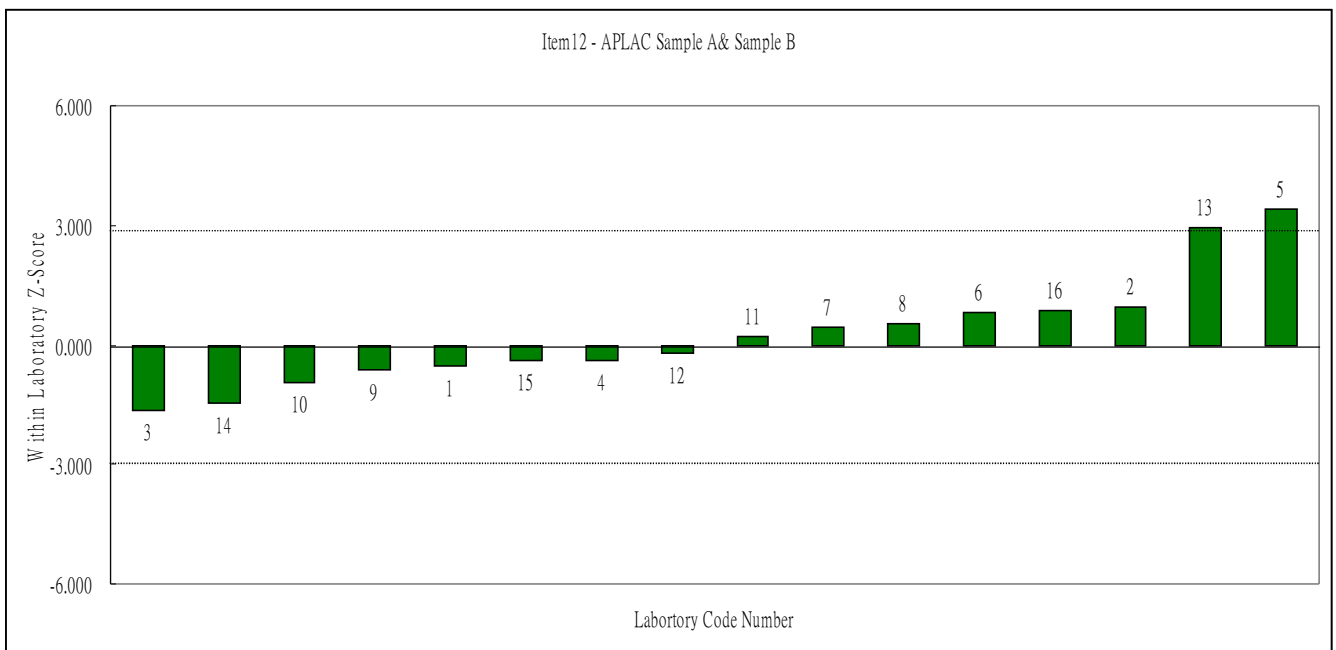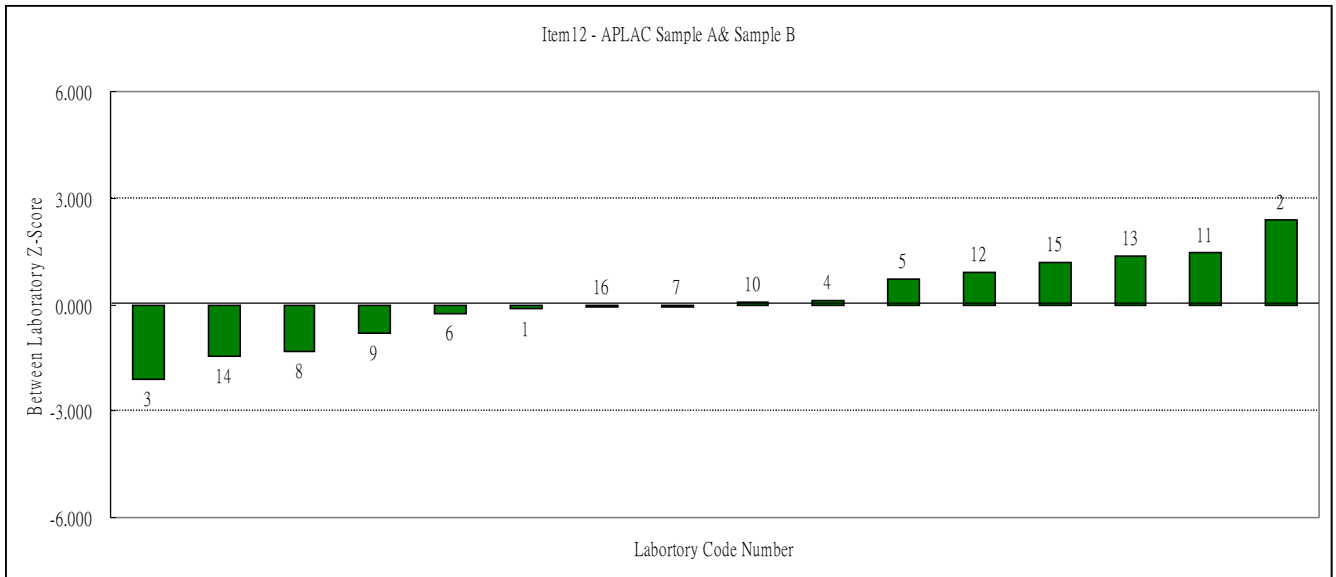

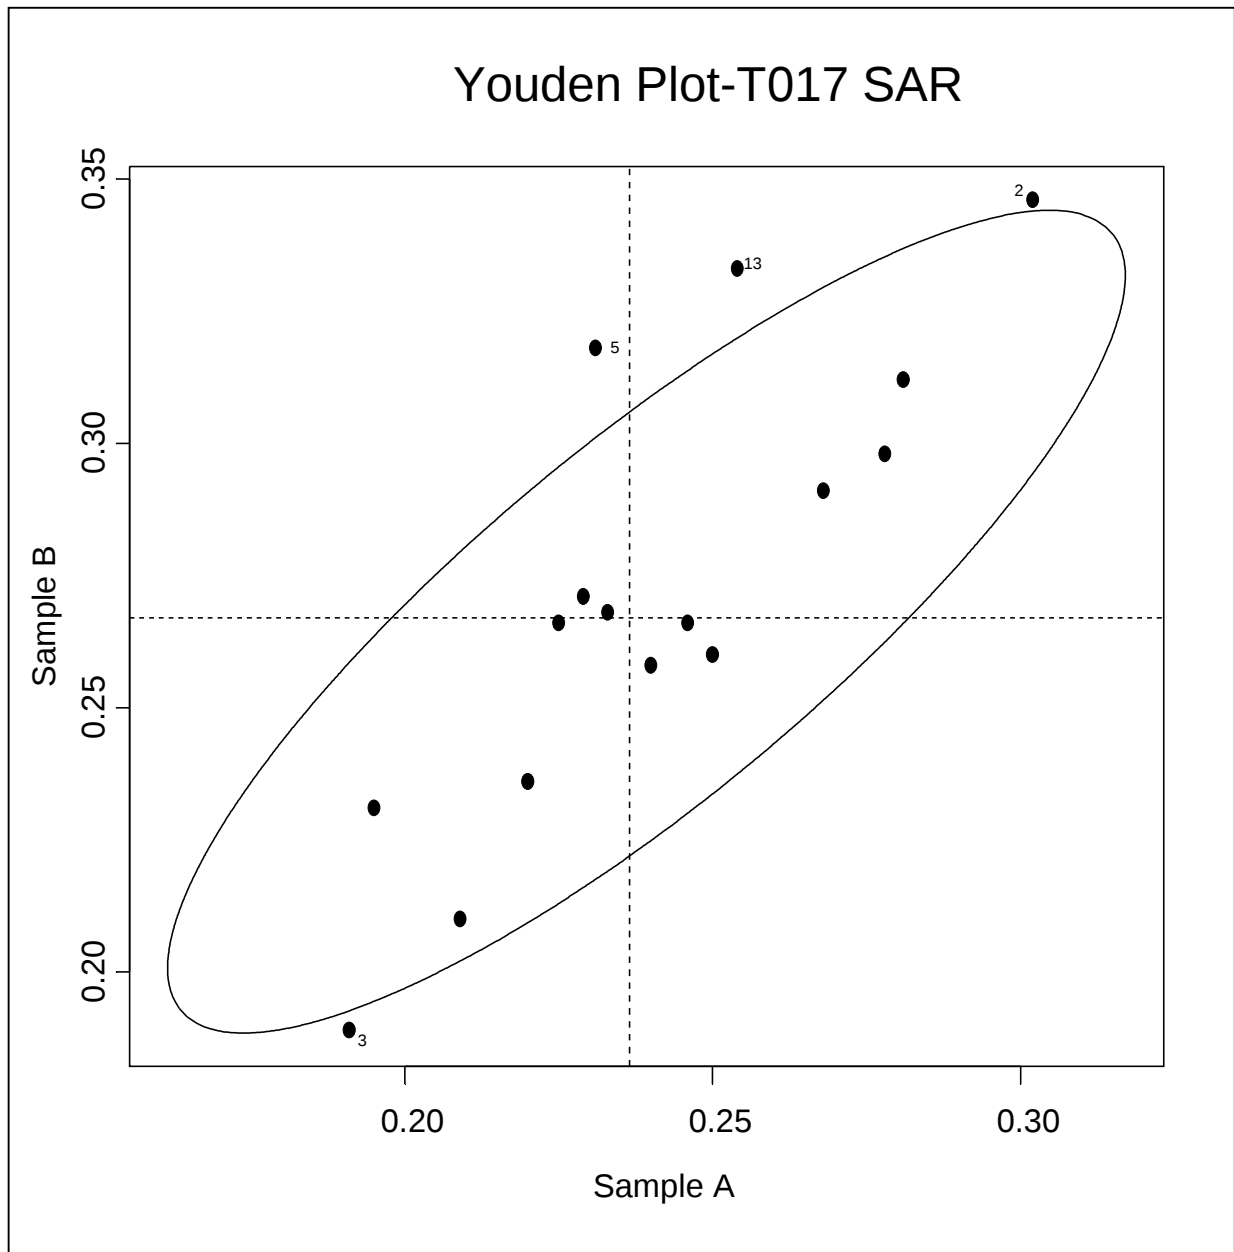

A13.1
Test methods and testing equipment

Lab Code No.	SAR Dosimetric Measurement System	Environment of Laboratory		Liquid Specifications	
		Temperature	Relative Humidity	Relative Dielectric Constant	Conductivity
		(°C)	(%)	Relative Dielectric Constant	σ (S/m)
1	DASY4	25.5	53	38.8	1.40
2	DASY3 (SPEAG)	21.2	48	40.2	1.40
3	MapSAR System (INDEXDAR)	21.0	49	41.0	1.70
4	DASY4	23.0	40	39.83	1.45
5	SPEAG DASY4	20-21	24-25	39.57(2004.12.21)/39.86(2004.12.22)	1.37(2004.12.21)/1.38(2004.12.22)
6	DASY4 Version 4.1 Build 47	22	62	39.57	1.405
7	SPEAG DASY4 V4.4 Build 3	21.6-21.7	61-63	39.1-39.8	1.40-1.44
8	DASY4	22(Sample A)/21(Sample B)	35 / 31	39.9 / 39.2	1.46 / 1.41
9	DASY4 System	24	56	39.62(Sample A)/39.05(Sample B)	1.3350(Sample A)/1.3444(Sample B)
10	ALSAS 10-Universal SAR Measurement System (Aprel)	22.9	55	38.8	1.37
11	DASY (SPEAG)	N/A	N/A	N/A	N/A
12	DASY4 System	22.3	48	41.20	1.402
13	DASY4 V4.2 Build 12	22.6	38.2	41.4 / 41.3 / 41.8	1.28 / 1.31 / 1.37
14	SARA2 by INDEXSAR	20	30	40	1.36
15	DASY4	21	60	39.9669	1.4080
16	DASY4	23.0	45	40.35	1.45

